

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Painted Sky Alpaca Farm/Mitchell Dickinson
95 Knight House Lane
Earleville MD 21919 USA

07/17/15

Test No: 907641


Animal and Sample Description

Animal Name: Viserion
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 32472677
Sample Location: Side (R)
Sample Date: 05/01/15
Age: 05/16/14

Laboratory Data

Mean Fiber Diameter: 16.9 microns
Standard Deviation: 3.1 microns
Coefficient of Variation: 18.5 %
Fibers Greater Than 30 microns: 0.5 %

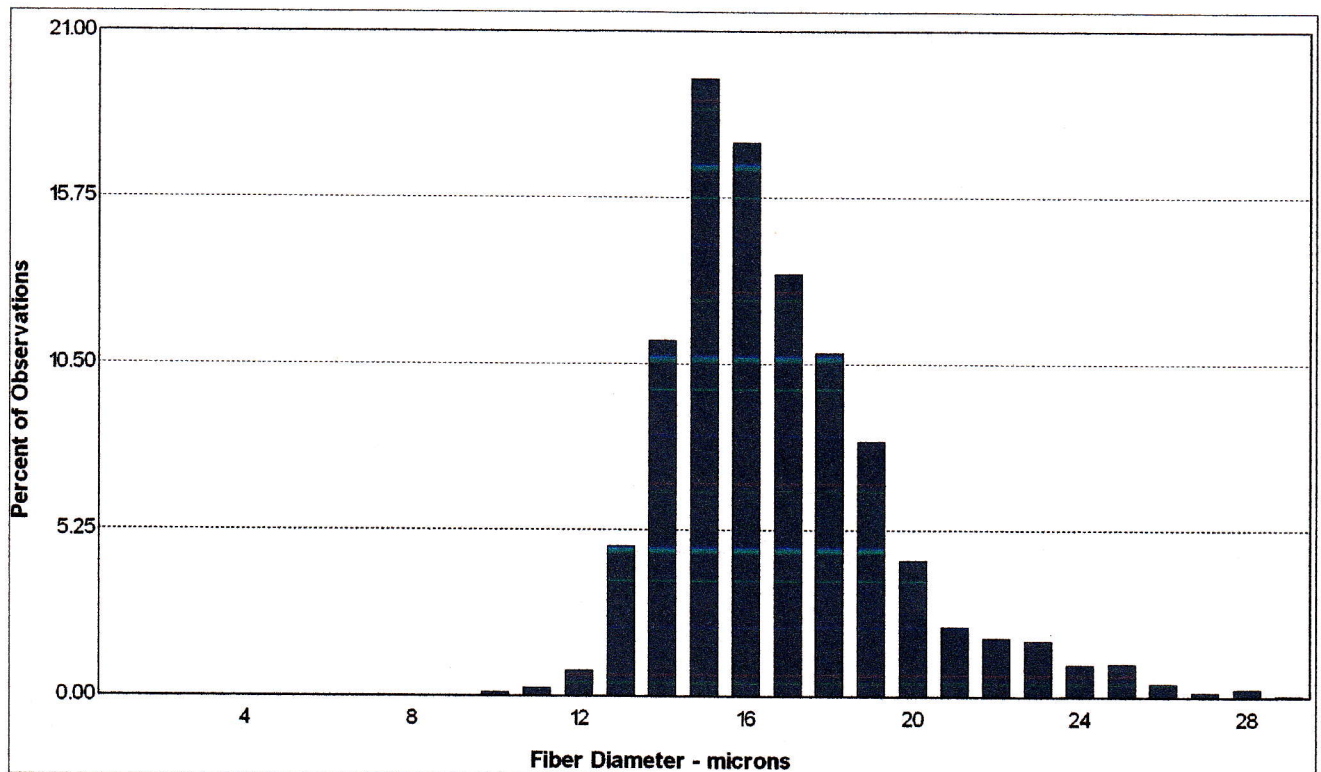

This Test Performed According to I.W.T.O Method 12