



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Andean Group/Glengary Farm/Patrick Cassese
2704 Slessman Drive
Plymouth OH 44865 USA

07/16/15

Test No: 906719


Animal and Sample Description

Animal Name: GGF Accoyo Bentley's Orabella
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/15/15
Age: 05/16/14

Laboratory Data

Mean Fiber Diameter:	16.2 microns	Spin Fineness:	16.2 microns
Standard Deviation:	3.8 microns	Mean Curvature (deg/mm):	40.9
Coefficient of Variation:	23.7 %	SD Curvature (deg/mm):	25.0
Fibers Greater Than 30 microns:	0.6 %	Comfort Factor:	99.4 %

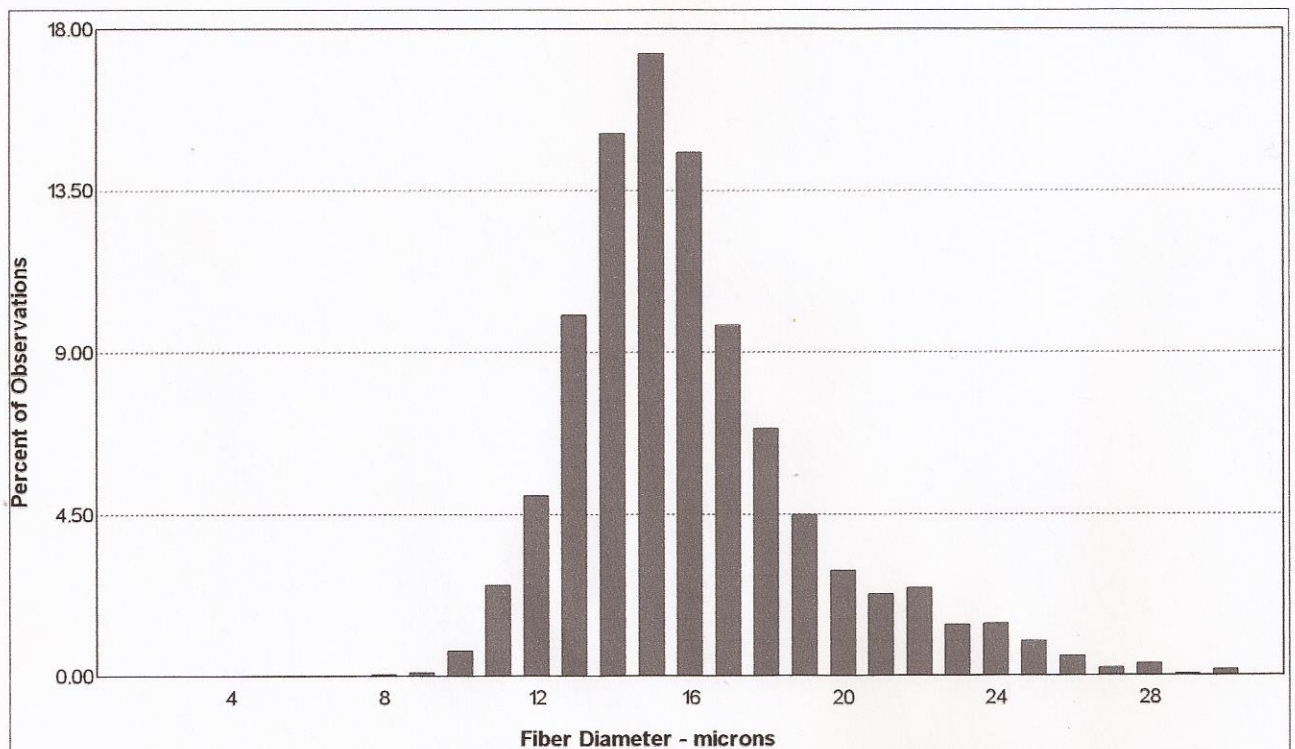

This Test Performed According to I.W.T.O Method 47