

Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Accoyo America/Dr Greg Mecklem
 12995 NW Bishop Road
 Hillsboro OR 97124 USA

03/06/13

Test No: 451018


Animal and Sample Description

Animal Name: Accoyo America Masai
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 32322446
Sample Location: Side
Sample Date: 02/15/13
Age: 03/13/12

Laboratory Data

Mean Fiber Diameter:	16.7 microns	Spin Fineness:	15.6 microns
Standard Deviation:	2.7 microns	Mean Curvature (deg/mm):	48.2
Coefficient of Variation:	16.0 %	SD Curvature (deg/mm):	26.1
Fibers Greater Than 30 microns:	0.2 %	Comfort Factor:	99.8 %
Medullated Fibers:	7.0 %		

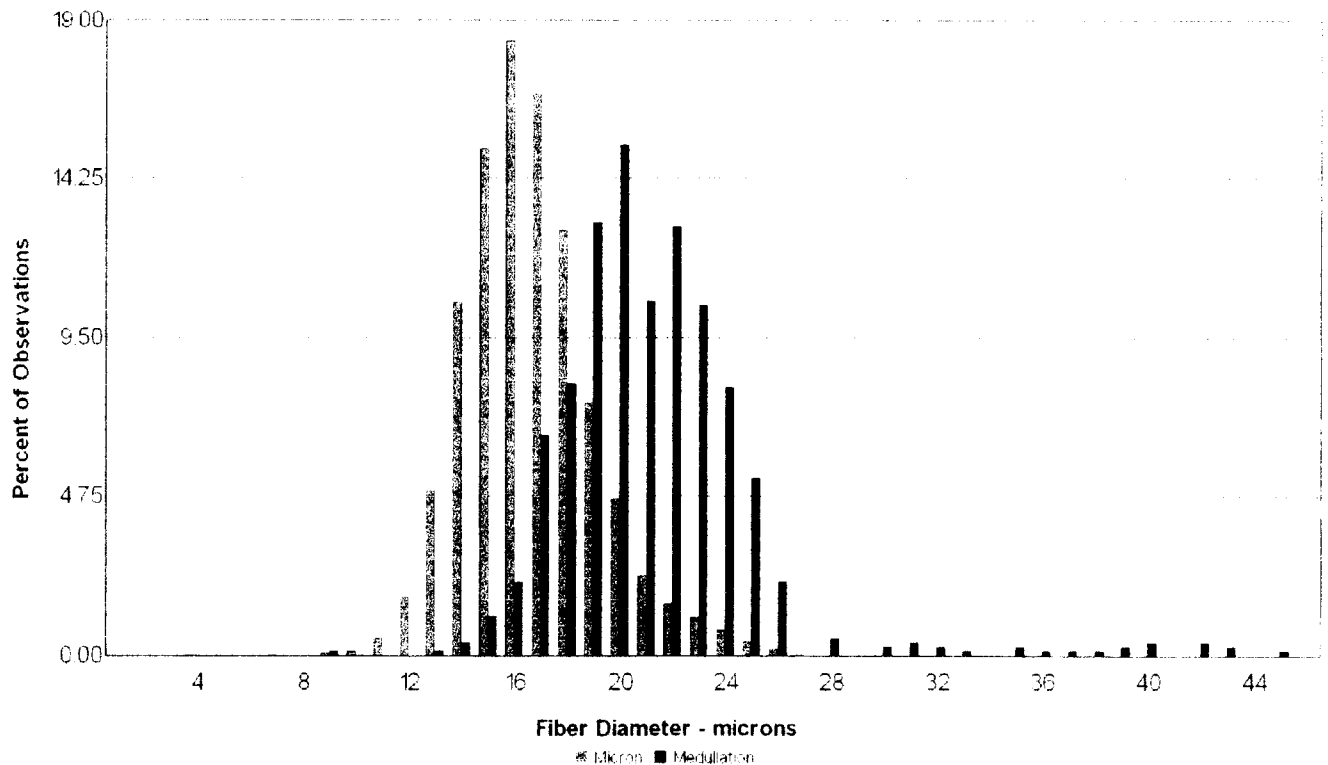

This Test Performed According to I.W.T.O Method 47