

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

EvenTyrGaard Alpacas/Gretchen Nygaard
17600 Fitch Ranch Rd
Sonora CA 95370 USA

10/05/12

Test No: 445136

Animal and Sample Description


Animal Name: GLR Picasso
Breed: Alpaca(Suri)
Sex: Male
Color: Dark Brown

Animal ID: 31115681
Sample Location: Side (R)
Sample Date: 05/11/12
Age: 10/11/09

RIGHT

Laboratory Data

Mean Fiber Diameter:	22.6 microns	Spin Fineness:	21.7 microns
Standard Deviation:	4.3 microns	Mean Curvature (deg/mm):	8.2
Coefficient of Variation:	19.2 %	SD Curvature (deg/mm):	10.4
Fibers Greater Than 30 microns:	4.7 %	Comfort Factor:	95.3 %

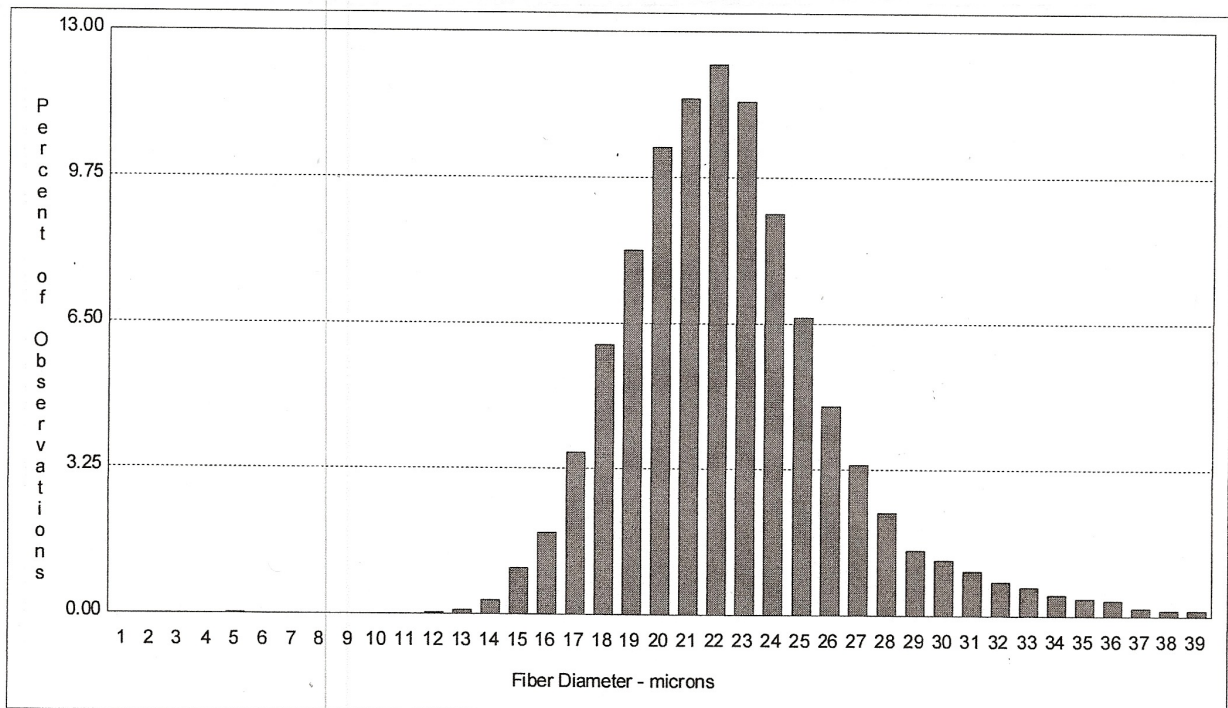

This Test Performed According to I.W.T.O Method 47