

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Mary's Alpaca, LLC/Mary Forte  
8080 Enon Church Road  
The Plains VA 20198

08/08/14

Test No: 489631


### Animal and Sample Description

**Animal Name:** Christina  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Brown

**Animal ID:** 32773040  
**Sample Location:** Side  
**Sample Date:** 05/02/14  
**Age:** 07/25/13

### Laboratory Data

**Mean Fiber Diameter:** 16.0 microns  
**Standard Deviation:** 3.0 microns  
**Coefficient of Variation:** 19.0 %  
**Fibers Greater Than 30 microns:** 0.4 %

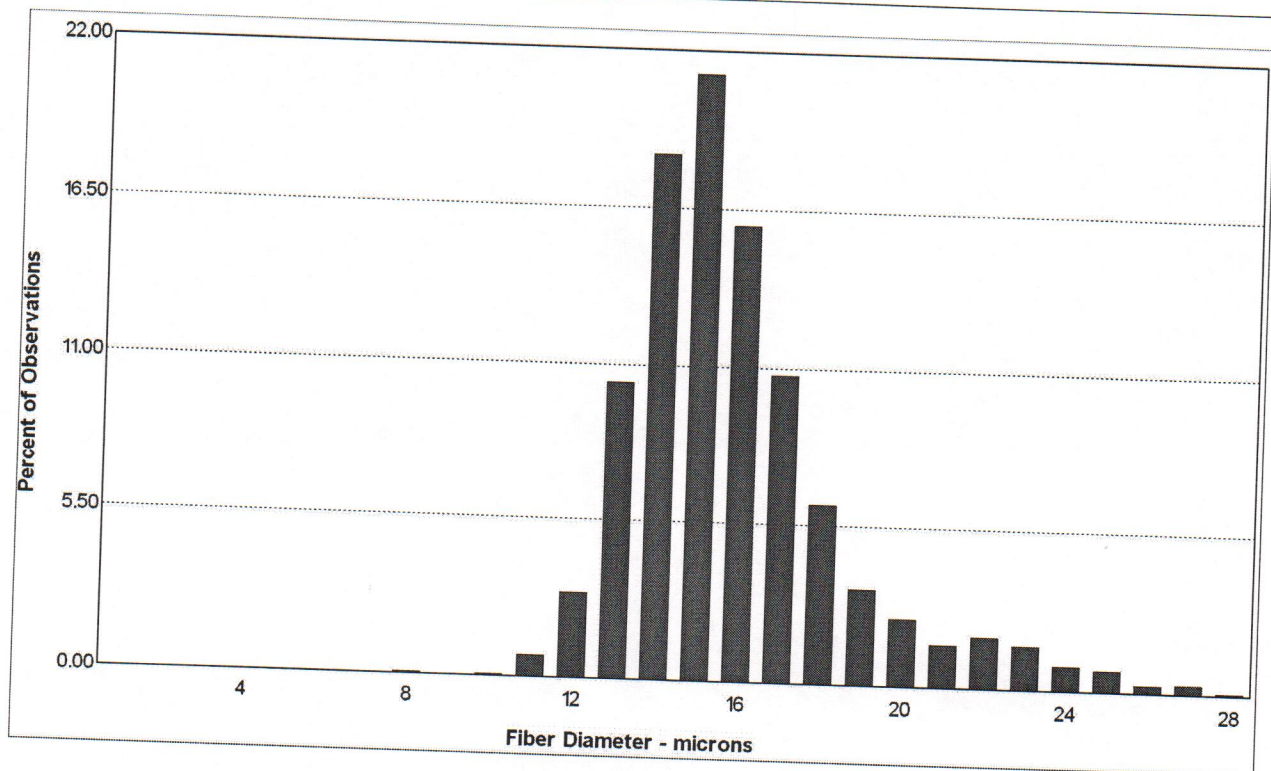

This Test Performed According to I.W.T.O Method 12