



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Mary's Alpaca, LLC/Mary Forte  
8080 Enon Church Road  
The Plains VA 20198

06/20/16

Test No: 922993


### Animal and Sample Description

**Animal Name:** Metrics  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 31998123  
**Sample Location:** Side  
**Sample Date:** 05/04/16  
**Age:** 06/18/10

### Laboratory Data

**Mean Fiber Diameter:** 18.3 microns  
**Standard Deviation:** 3.7 microns  
**Coefficient of Variation:** 19.9 %  
**Fibers Greater Than 30 microns:** 0.8 %

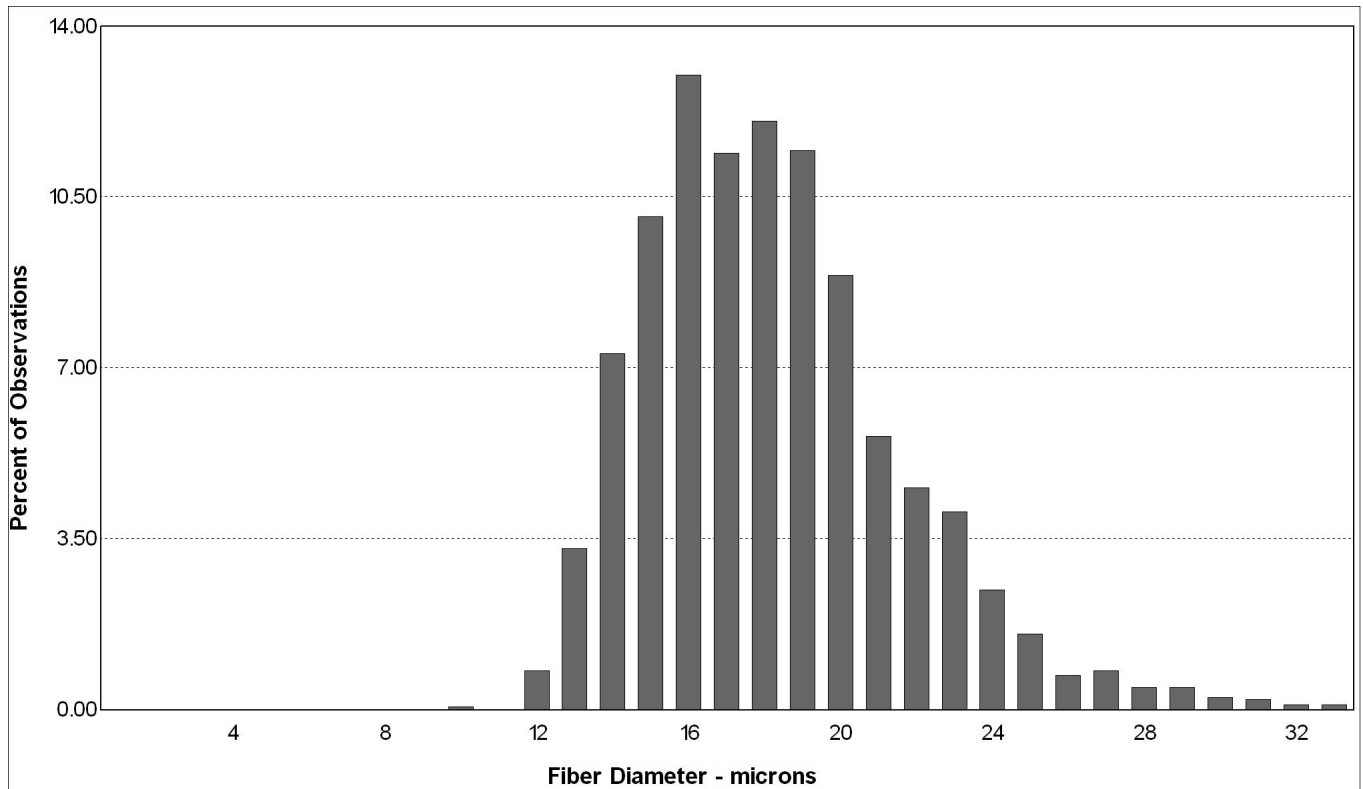

This Test Performed According to I.W.T.O Method 12