



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Cabin View Alpacas/Christine & David Houseworth
9435 Congress St Ext
Trumansburg NY 14886 USA

06/30/16

Test No: 925629


Animal and Sample Description

Animal Name: Drifter of Cabin View
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Brown

Animal ID: 32702873
Sample Location: Mid Side
Sample Date: 05/21/16
Age: 08/28/15

Laboratory Data

Mean Fiber Diameter: 19.7 microns
Standard Deviation: 3.4 microns
Coefficient of Variation: 17.3 %
Fibers Greater Than 30 microns: 1.1 %

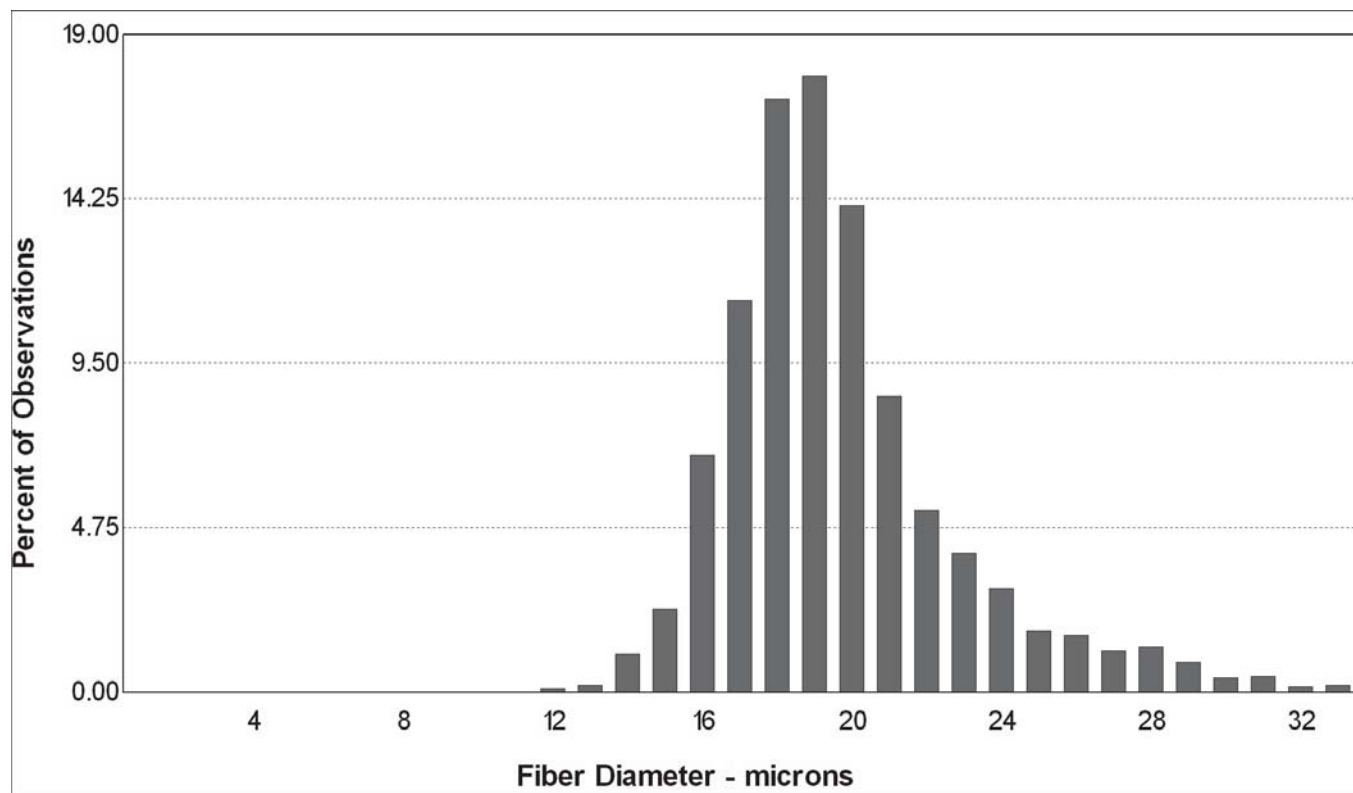

This Test Performed According to I.W.T.O Method 12