

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Golden Pine Alpacas/Pat & Barbara Patterson  
163 Golden Pine  
Goldendale WA 98620

04/28/17

Test No: 941137


### Animal and Sample Description

**Animal Name:** Golden Pine's Victoria  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Dark Fawn

**Animal ID:** 32728743  
**Sample Location:** Side  
**Sample Date:** 04/04/17  
**Age:** 09/25/13

### Laboratory Data

**Mean Fiber Diameter:** 21.8 microns  
**Standard Deviation:** 4.2 microns  
**Coefficient of Variation:** 19.2 %  
**Fibers Greater Than 30 microns:** 3.8 %

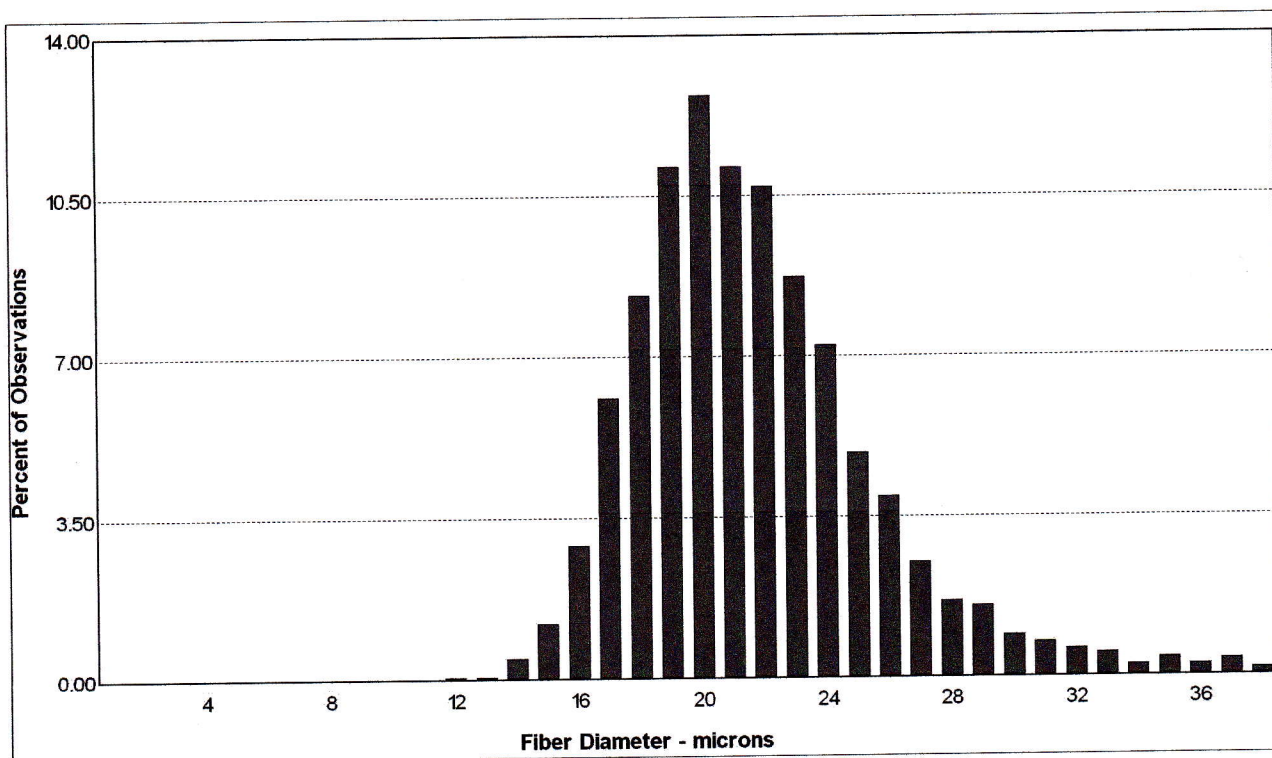

This Test Performed According to I.W.T.O Method 12