



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Dreamcatcher Alpacas, LLC/Patty Jensen
618 34 1/2 Rd
Clifton CO 81520-8415

07/05/17

Test No: 944722


Animal and Sample Description

Animal Name: Dreamcatcher Peruvian Regis
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 31758239
Sample Location: Side (R)
Sample Date: 05/07/17
Age: 08/29/09

Laboratory Data

Mean Fiber Diameter: 22.9 microns
Standard Deviation: 5.0 microns
Coefficient of Variation: 21.7 %
Fibers Greater Than 30 microns: 7.0 %

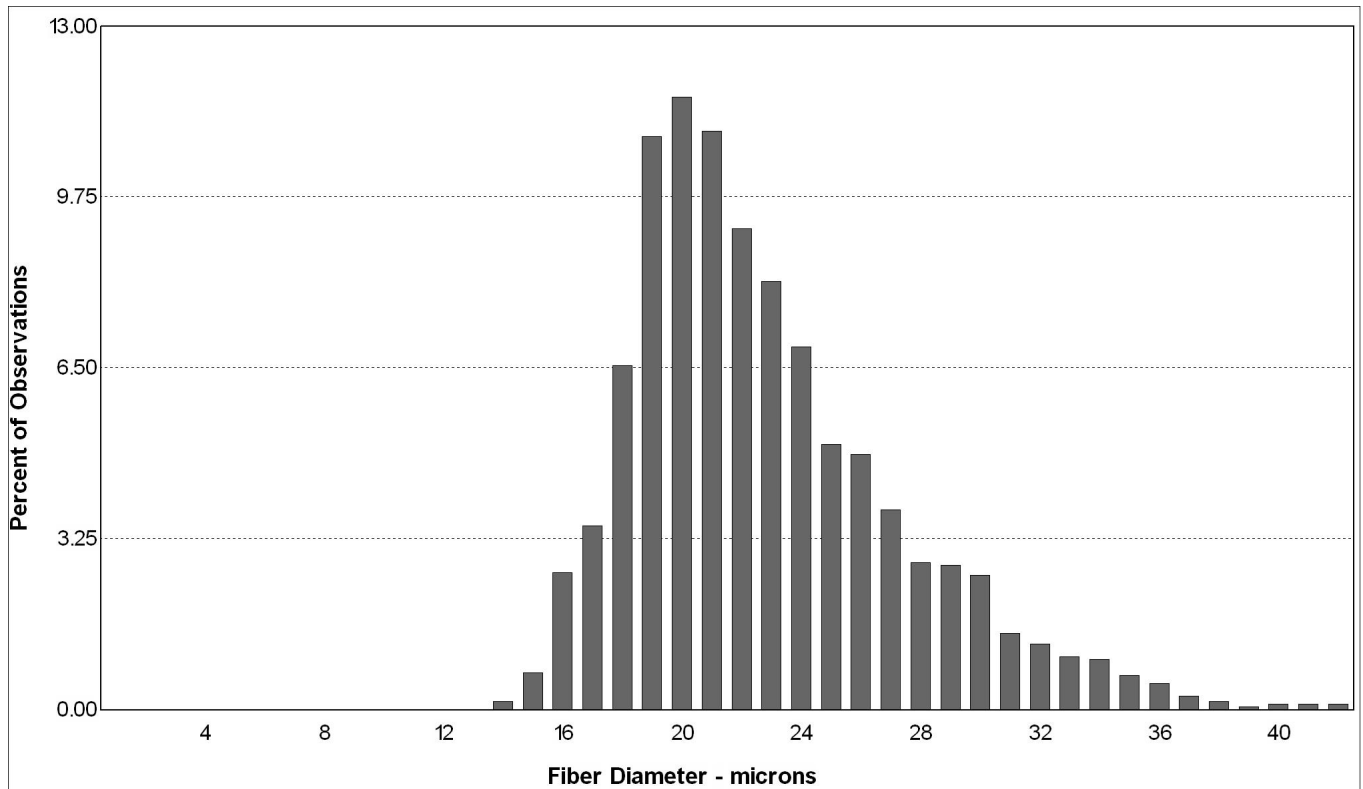

This Test Performed According to I.W.T.O Method 12