Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Sky Ridge Alpacas/Stacie Chavez
58150 Highway 197
Tygh Valley OR 97063

Date: 06/29/16

Test No: 925238

Animal and Sample Description

Animal Name:	Albuquerque Alpacas Maddie	**Animal ID:**	32644777
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	05/24/16
Color:	White	**Age:**	10/02/13

Laboratory Data

Mean Fiber Diameter:	17.4	microns	**Fibers Greater Than 30 microns:**	0.7	%
Standard Deviation:	4.1	microns	**Comfort Factor:**	99.3	%
Coefficient of Variation:	23.6	%	**Mean Curvature:**	50.2	deg/mm
Spin Fineness:	17.3	microns	**SD Curvature:**	26.2	deg/mm

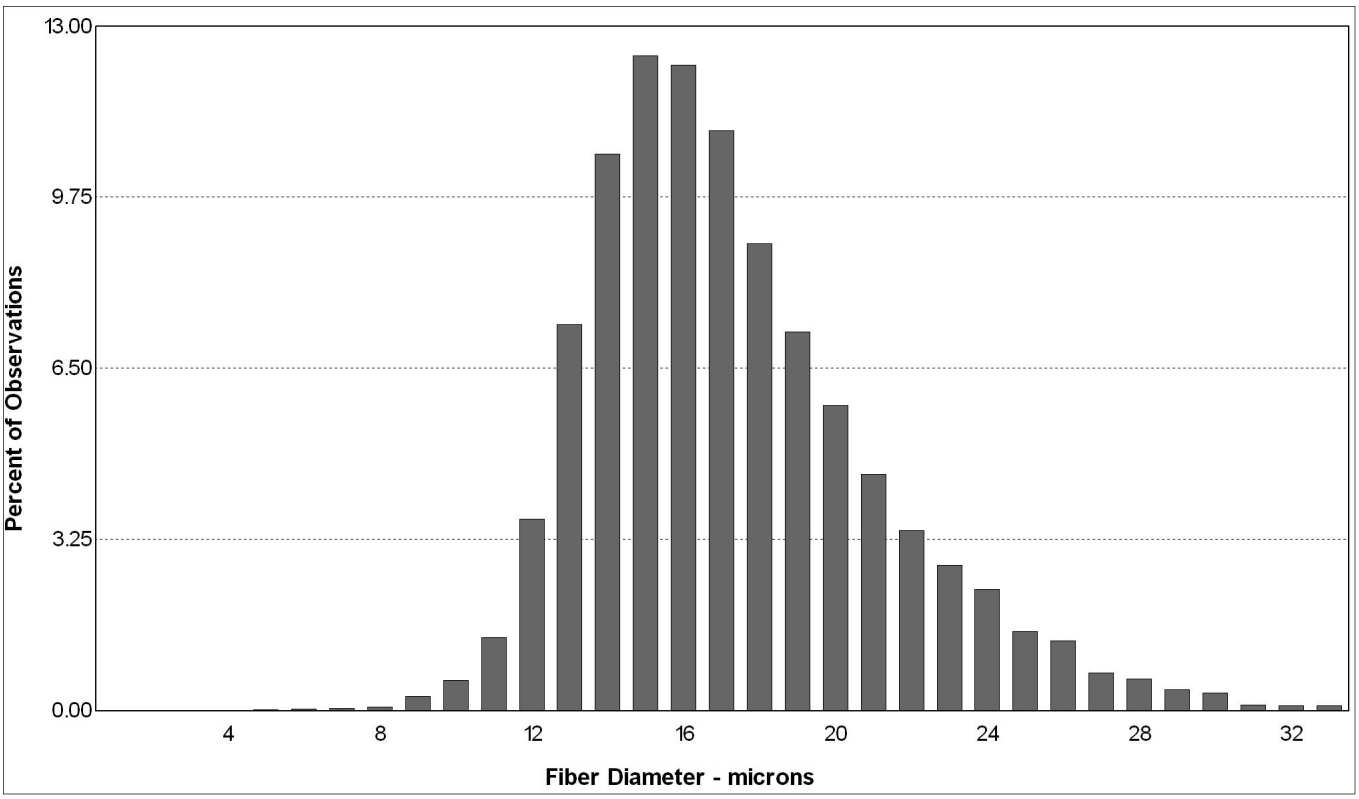

This Test Performed According to I.W.T.O Method 47