



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Nueva Dia Alpacas/Theresa Kaiser
7123 Reinneck Rd
Belleville IL 62221 USA

Date: 06/09/17

Test No: 942601


Animal and Sample Description

Animal Name: Quicksand's Smoked Quartz
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Brown

Animal ID: 32845969
Sample Location: Side
Sample Date: 04/15/17
Age: 07/08/15

Laboratory Data

Mean Fiber Diameter:	20.5 microns	Fibers Greater Than 30 microns:	1.6 %
Standard Deviation:	3.7 microns	Comfort Factor:	98.4 %
Coefficient of Variation:	18.2 %	Mean Curvature:	31.7 deg/mm
Spin Fineness:	19.5 microns	SD Curvature:	22.8 deg/mm

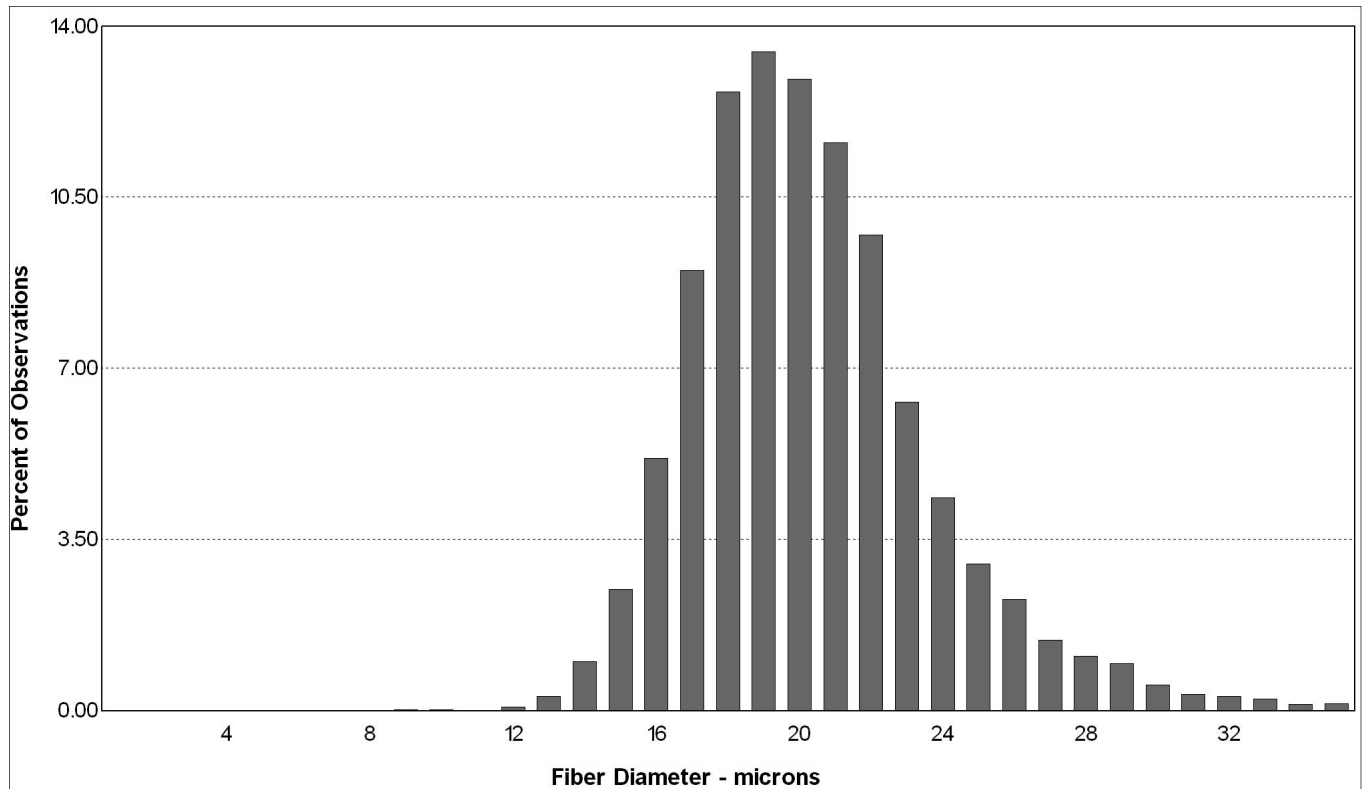

This Test Performed According to I.W.T.O Method 47