



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Owl Ridge Alpacas/Jodie Vanselow
7842 Hall Rd
Interlaken NY 14847 USA

05/17/16

Test No: 921224


Animal and Sample Description

Animal Name: Owl Ridge Mystique
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/28/16
Age: 06/24/15

Laboratory Data

Mean Fiber Diameter: 17.5 microns
Standard Deviation: 3.6 microns
Coefficient of Variation: 20.6 %
Fibers Greater Than 30 microns: 0.6 %

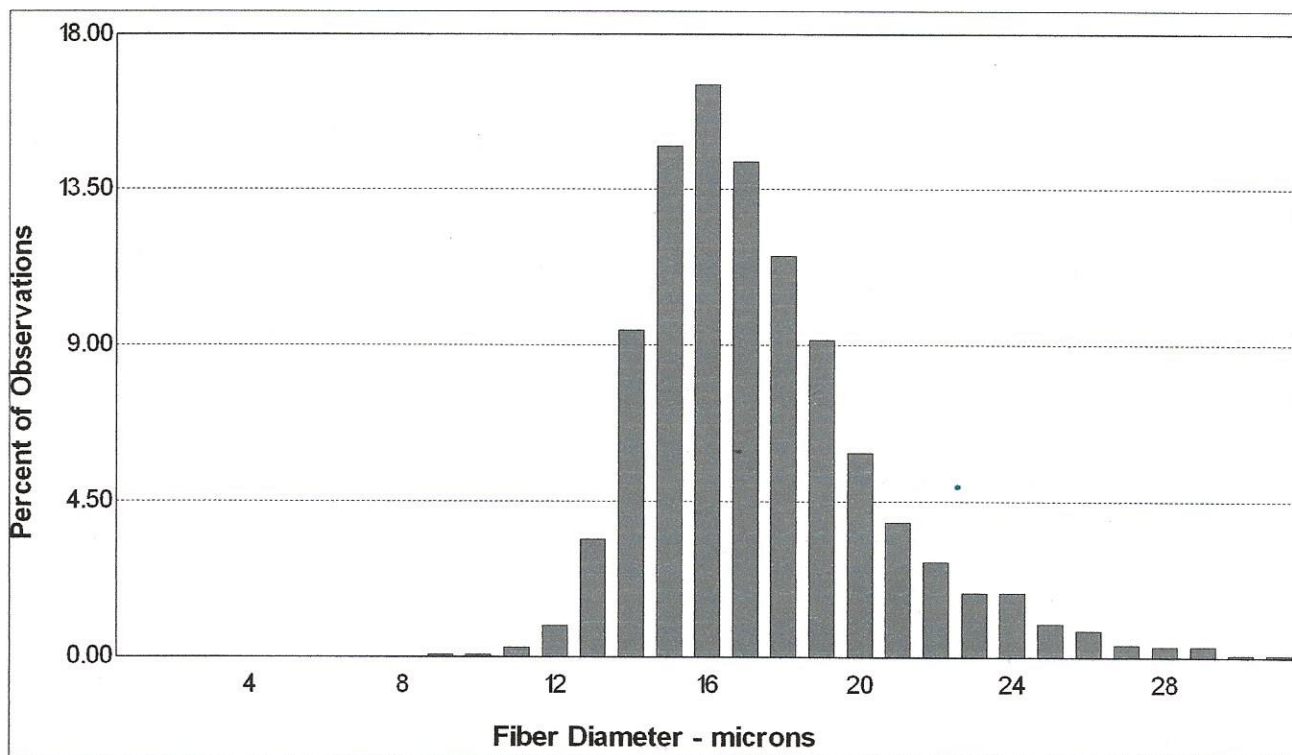

This Test Performed According to I.W.T.O Method 12