



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Hasselbring's Harmony Ranch/Patty Hasselbring  
29049 Davis Road  
Concordia MO 64020 USA


Date: 08/11/17  
Shear ID: 145108  
Test No: 946921

### Animal and Sample Description

<b>Animal Name:</b>	WLK Nefa Tari	<b>Date of Birth (Age):</b>	06/28/10
<b>ARI #:</b>	31977968	<b>Sample Location:</b>	Side
<b>Breed:</b>	Alpaca(Huacaya)	<b>Sample Date:</b>	05/19/17
<b>Sex:</b>	Female	<b>Previous Shear Date:</b>	05/21/16
<b>Color:</b>	Dark Silver Grey	<b>Total Fleece Wt (lbs):</b>	4.00

### Laboratory Data

<b>Mean Fiber Diameter:</b>	30.9 microns	<b>Mean Staple Length:</b>	114.4 mm
<b>Standard Deviation:</b>	7.6 microns	<b>Length Standard Deviation:</b>	3.1 mm
<b>Coefficient of Variation:</b>	24.4 %	<b>Length Coefficient of Variation:</b>	2.7 %
<b>Spin Fineness:</b>	31.0 microns	<b>Mean Curvature:</b>	10.3 deg/mm
<b>Fibers Greater Than 30 microns:</b>	42.4 %	<b>SD Curvature:</b>	13.0 deg/mm
<b>Comfort Factor:</b>	57.6 %		

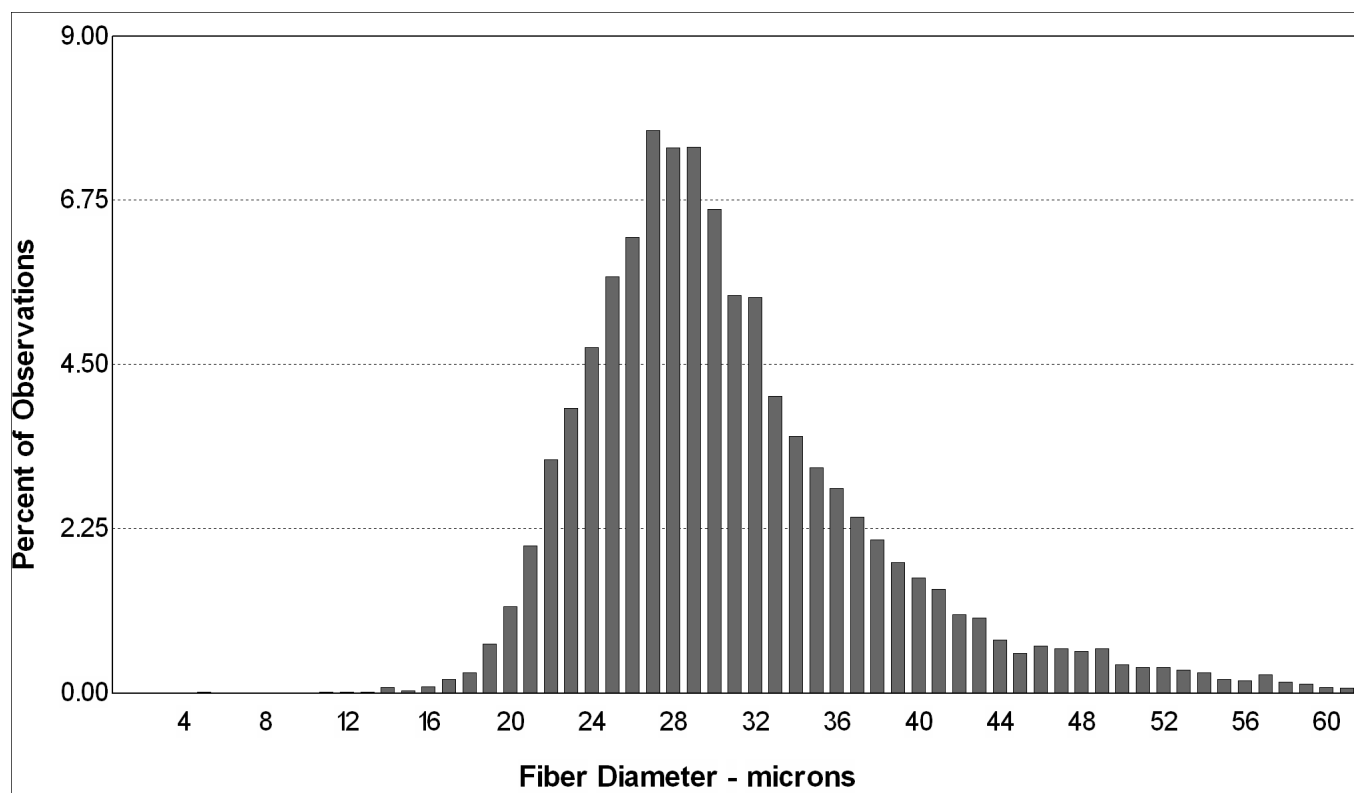

This Test Performed According to I.W.T.O Method 47