

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Breezy Meadows Alpacas/Charlene Arnold
2061 Moravia Venice Townline Rd
Moravia NY 13118 USA

08/02/17

Test No: 947950


Animal and Sample Description

Animal Name: Miss Molly
Breed: Alpaca(Huacaya)
Sex: Female
Color: XXXXX

Animal ID: 32783742
Sample Location: Side
Sample Date: 05/10/17
Age: 10/03/16

Laboratory Data

Mean Fiber Diameter: 21.8 microns
Standard Deviation: 3.9 microns
Coefficient of Variation: 17.8 %
Fibers Greater Than 30 microns: 3.0 %

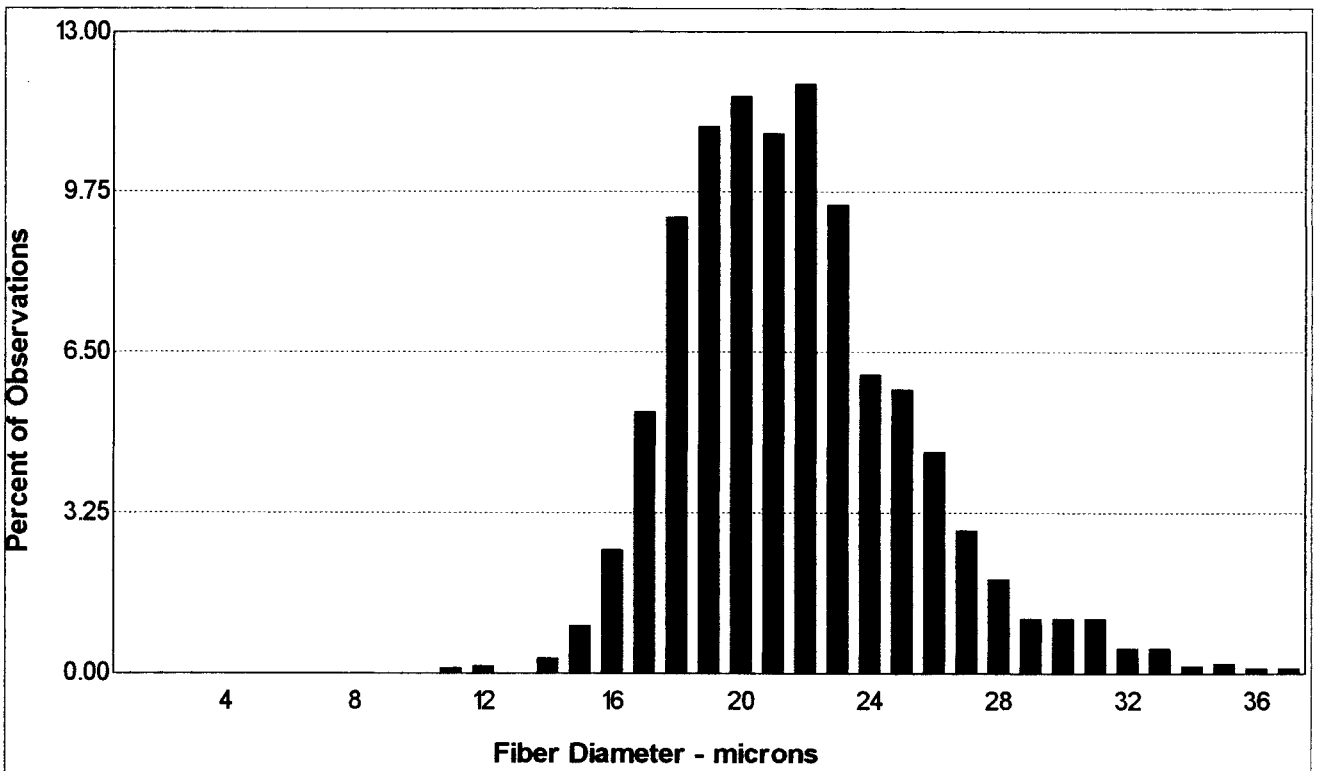

This Test Performed According to I.W.T.O Method 12