



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Delphi Alpacas/Linda Bat
P.O. Box 9
Coaldale CO 81222

05/29/18

Test No: 960392


Animal and Sample Description

Animal Name: Amerilly 2017
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Silver Grey

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/17/17
Age: XXXXX

Laboratory Data

Mean Fiber Diameter: 13.9 microns
Standard Deviation: 3.1 microns
Coefficient of Variation: 22.1 %
Fibers Greater Than 30 microns: 0.3 %

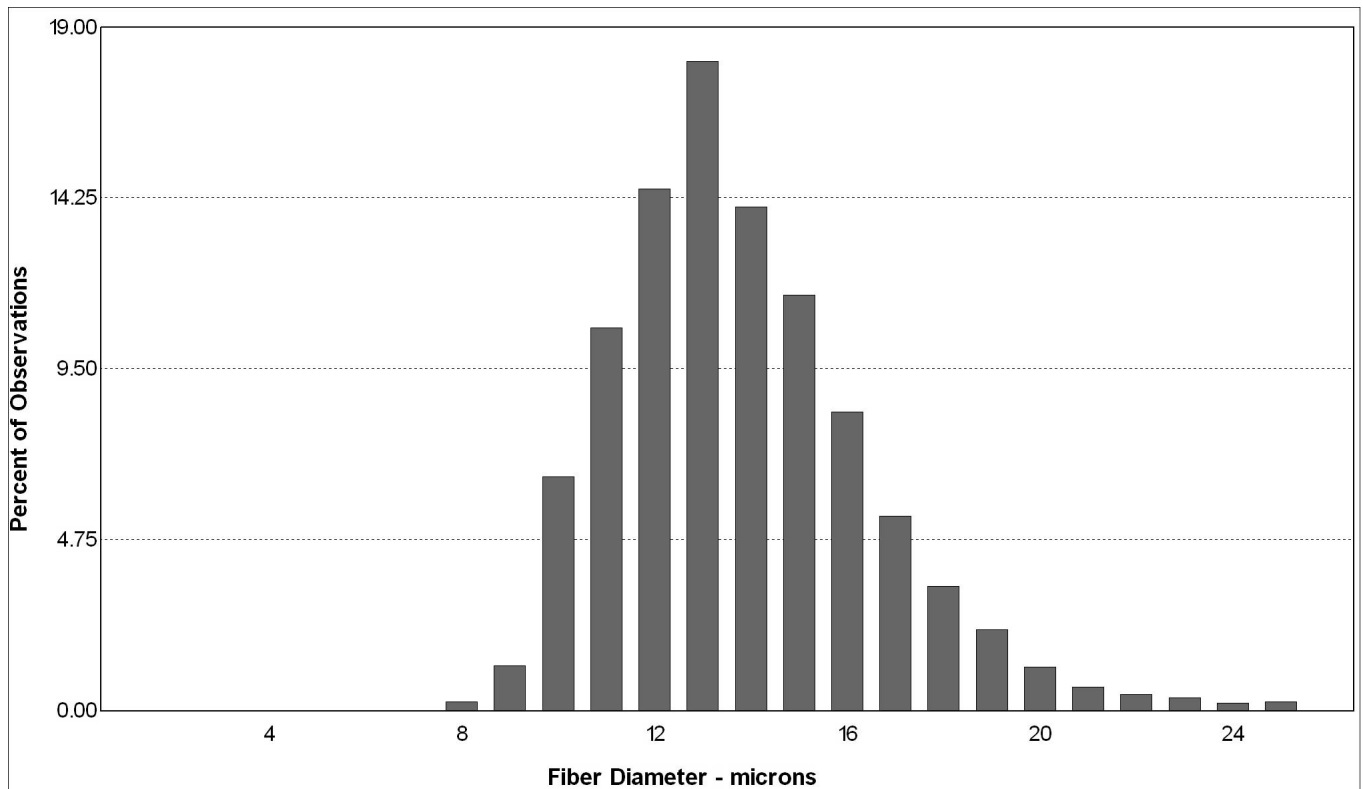

This Test Performed According to I.W.T.O Method 12