

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Claddagh Farm/Sarah Lamanna
6905 Stebbins Rd
LaFayette NY 13084-9408

Date: 03/29/18

Test No: 957718


Animal and Sample Description

Animal Name: Shooting Star's Sterling
Breed: Alpaca(Huacaya)
Sex: Male
Color: White w/Black

Animal ID: 31349291
Sample Location: Mid Side
Sample Date: 03/25/18
Age: 08/11/08

Laboratory Data

Mean Fiber Diameter:	27.8 microns	Fibers Greater Than 30 microns:	21.8 %
Standard Deviation:	4.8 microns	Comfort Factor:	78.2 %
Coefficient of Variation:	17.4 %	Mean Curvature:	27.7 deg/mm
Spin Fineness:	26.2 microns	SD Curvature:	17.6 deg/mm

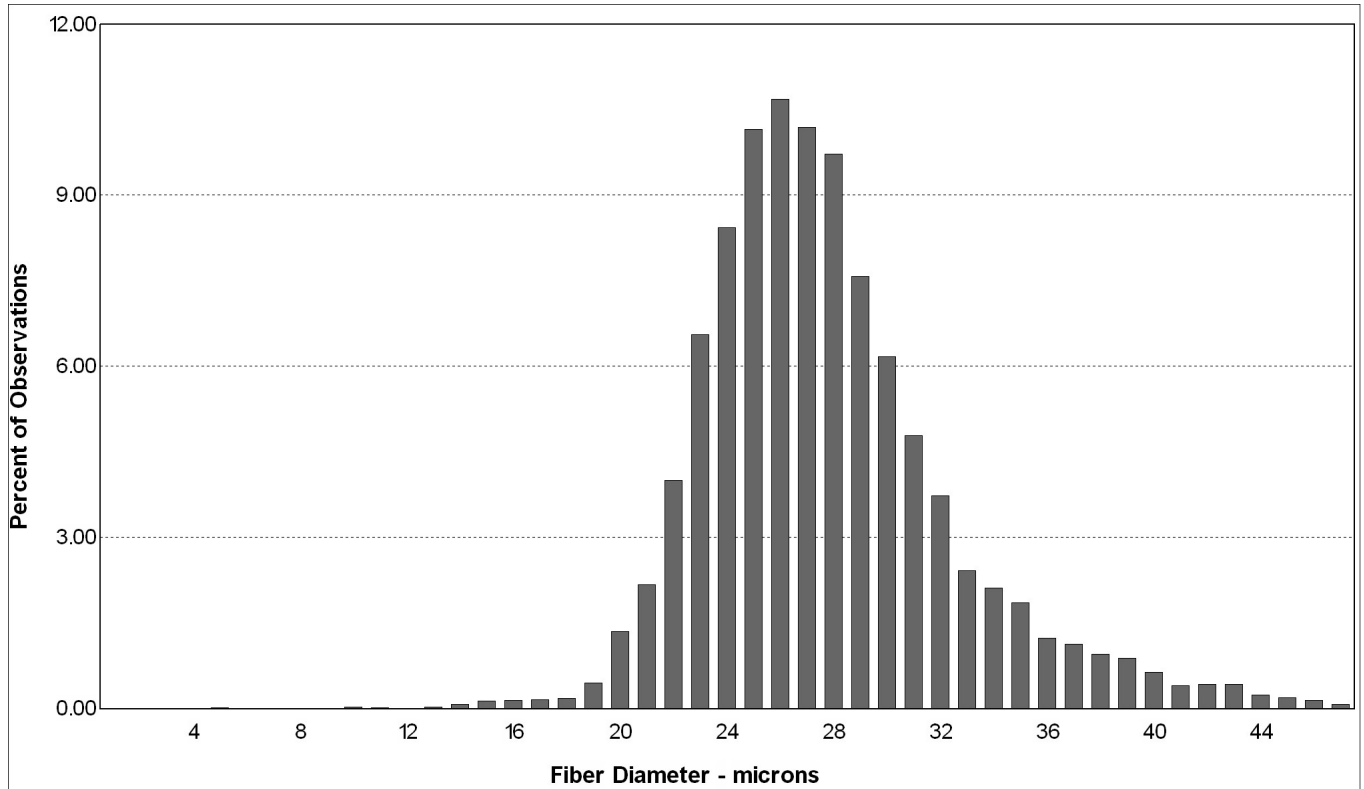

This Test Performed According to I.W.T.O Method 47