

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

B I Bar Ranch/Julie M Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

06/16/18

Test No: 961855


Animal and Sample Description

Animal Name: BIR's Paradox Stout
Breed: Alpaca(Suri)
Sex: Male
Color: DB

Animal ID: 32560466
Sample Location: Side (R)
Sample Date: 06/01/18
Age: 07/20/14

Laboratory Data

Mean Fiber Diameter: 22.9 microns
Standard Deviation: 3.7 microns
Coefficient of Variation: 16.0 %
Fibers Greater Than 30 microns: 3.6 %

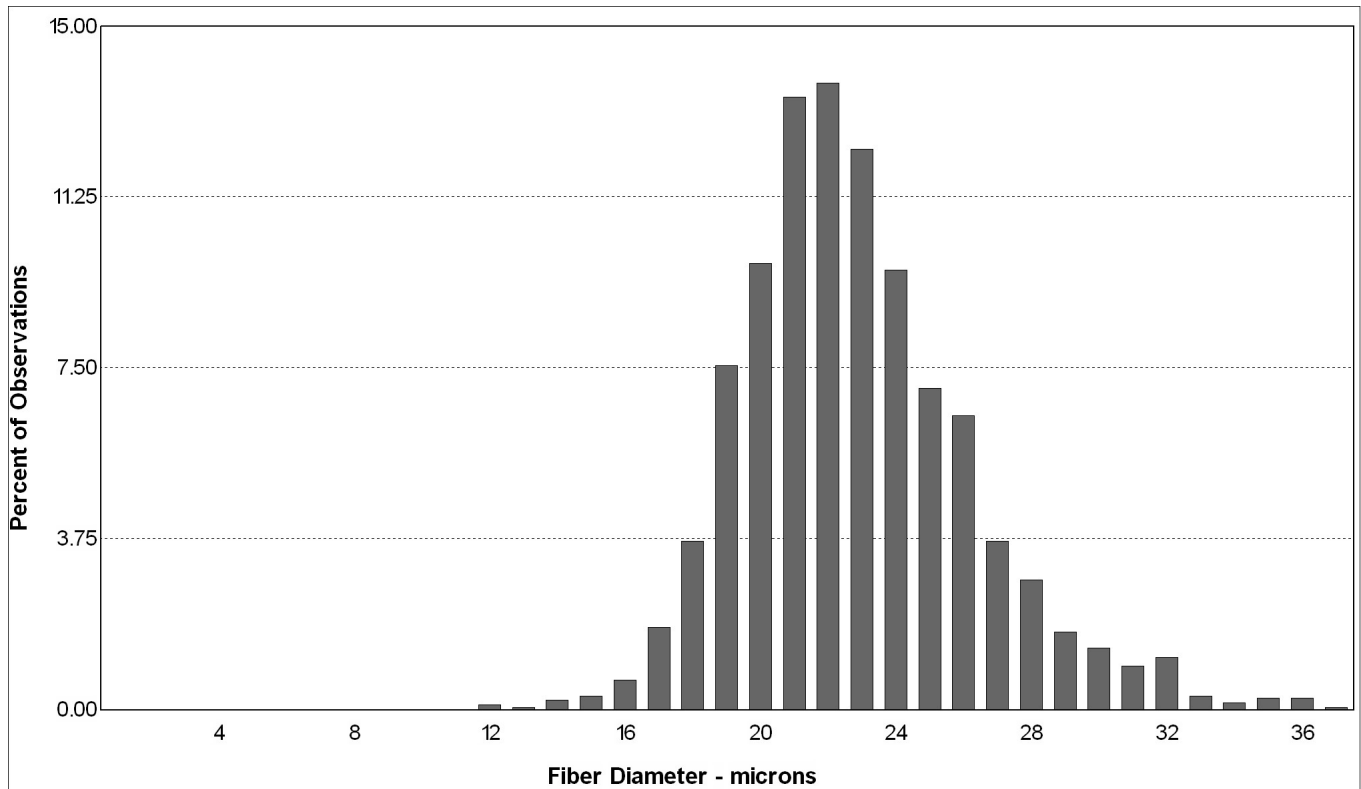

This Test Performed According to I.W.T.O Method 12