

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Golden Pine Alpacas/Pat & Barbara Patterson
163 Golden Pine
Goldendale WA 98620

04/28/17

Test No: 941139


Animal and Sample Description

Animal Name: Antonio of Golden Pine
Breed: Alpaca(Huacaya)
Sex: Male
Color: True Black

Animal ID: 32304619
Sample Location: Side
Sample Date: 04/04/17
Age: 06/22/11

Laboratory Data

Mean Fiber Diameter: 20.9 microns
Standard Deviation: 4.4 microns
Coefficient of Variation: 21.1 %
Fibers Greater Than 30 microns: 4.5 %

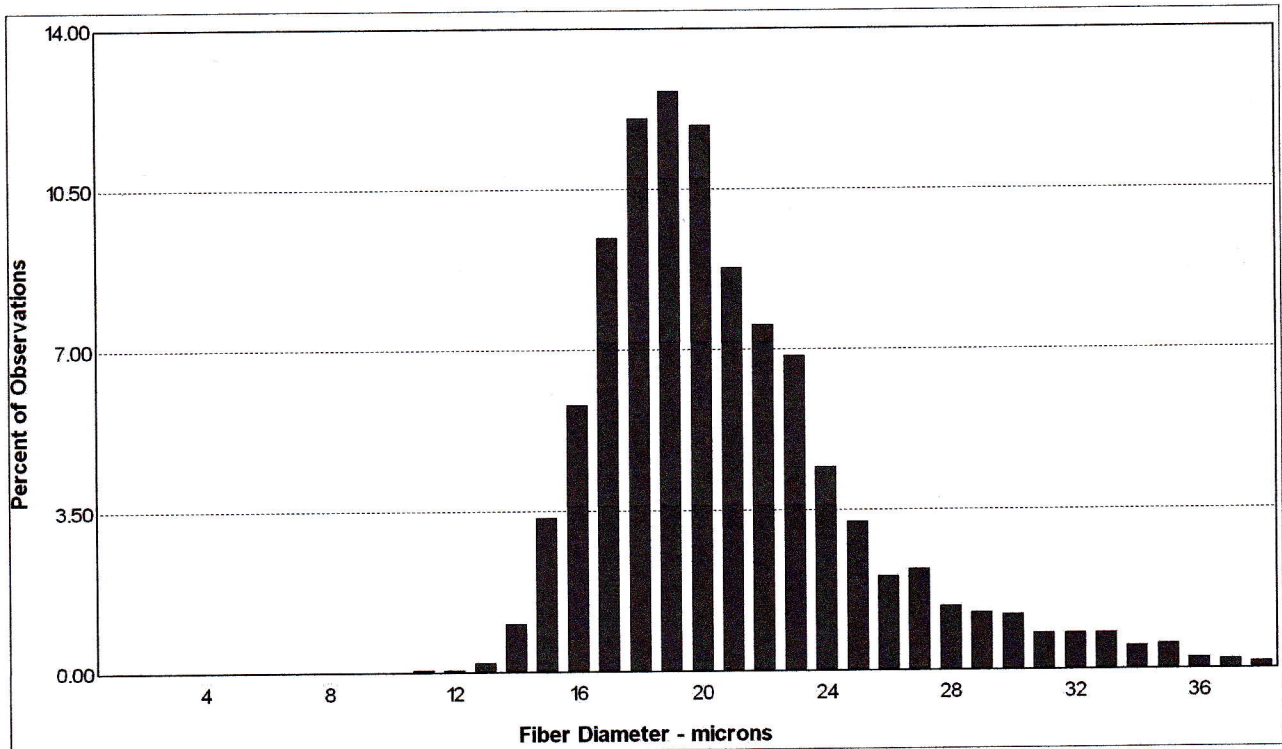

This Test Performed According to I.W.T.O Method 12