



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Hopeful Hills Ranch/Jane Fauskee
30577 N Scandi Dr
Glenwood MN 56334-9512 USA

03/13/18

Test No: 956988


Animal and Sample Description

Animal Name: Tux
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Silver Grey

Animal ID: 32634198
Sample Location: Side
Sample Date: 04/28/17
Age: 05/18/14

Laboratory Data

Mean Fiber Diameter: 16.7 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 27.2 %
Fibers Greater Than 30 microns: 2.1 %

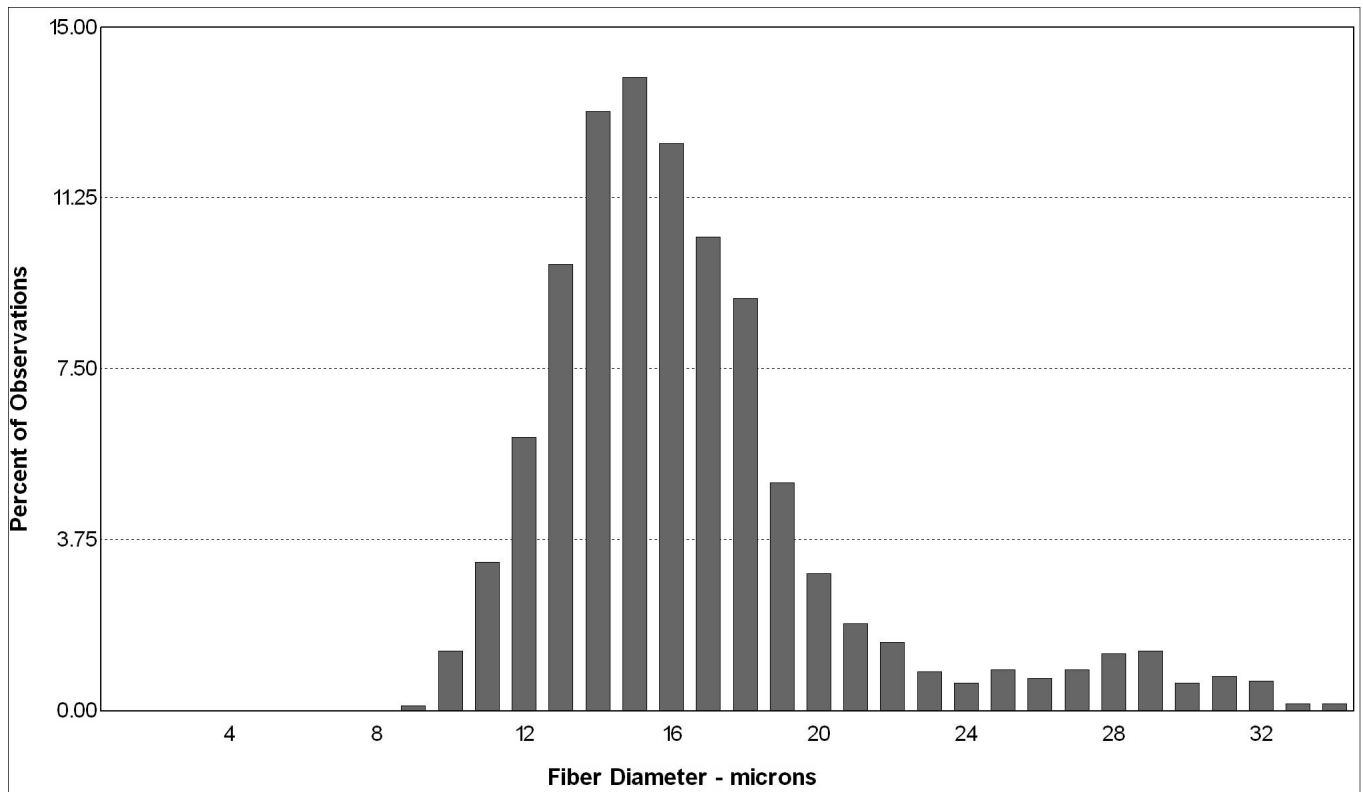

This Test Performed According to I.W.T.O Method 12