Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

The Alpacas of Spring Acres/Dr. Pam Walker DMV
3370 Big B Rd
Zanesville OH 43701 USA

05/15/18

Test No: 959573

Animal and Sample Description

Animal Name:	CHFA Accoyo Lady Chatterly	**Animal ID:**	1434446
Breed:	Alpaca(Suri)	**Sample Location:**	Blanket
Sex:	Female	**Sample Date:**	04/28/18
Color:	White	**Age:**	04/06/04

Laboratory Data

Mean Fiber Diameter:	25.7	microns
Standard Deviation:	5.0	microns
Coefficient of Variation:	19.3	%
Fibers Greater Than 30 microns:	15.1	%

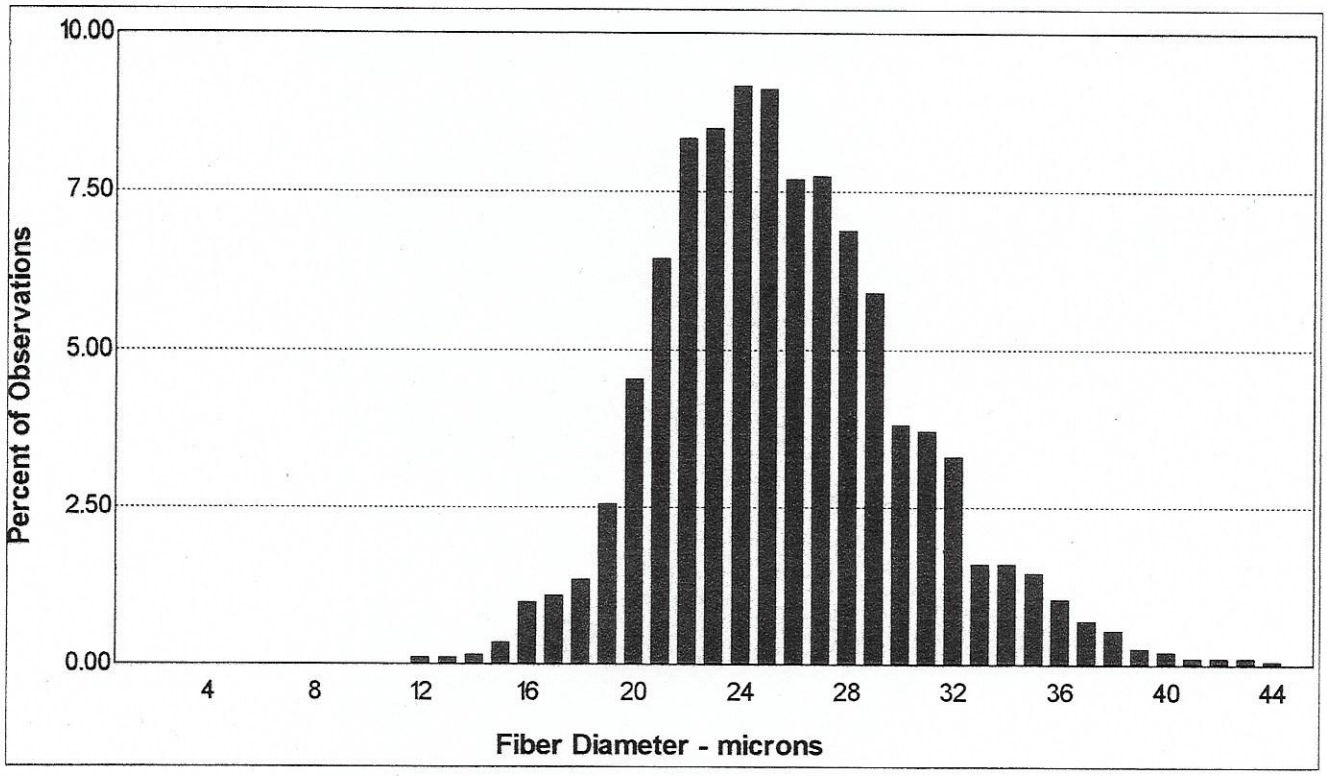

This Test Performed According to I.W.T.O Method 12