

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Indian Valley Alpaca Ranch/Teresa Hull  
1066 Grays Creek Rd  
Indian Valley ID 83632 USA

Date: 08/05/18

Test No: 965897


### Animal and Sample Description

**Animal Name:** Atara Royal Bronze  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Dark Fawn

**Animal ID:** 31812528  
**Sample Location:** Side  
**Sample Date:** 05/05/18  
**Age:** 08/26/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	18.6 microns	<b>Fibers Greater Than 30 microns:</b>	3.6 %
<b>Standard Deviation:</b>	5.3 microns	<b>Comfort Factor:</b>	96.4 %
<b>Coefficient of Variation:</b>	28.6 %	<b>Mean Curvature:</b>	44.9 deg/mm
<b>Spin Fineness:</b>	19.4 microns	<b>SD Curvature:</b>	28.3 deg/mm

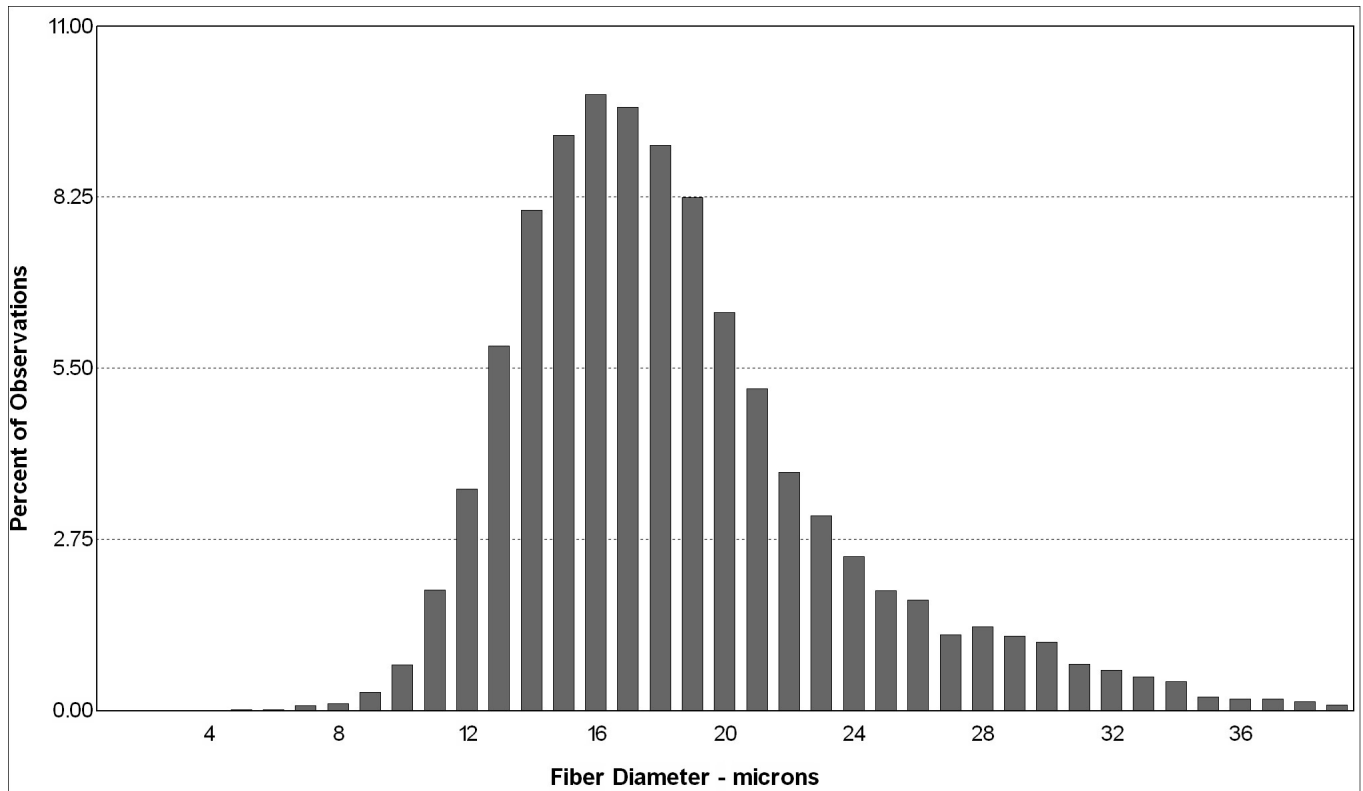

This Test Performed According to I.W.T.O Method 47