



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Fiber Meadows Alpacas/Dean & Pamela Hiestand  
26417 Minkler Rd  
Sedro Woolley WA 98284 USA

02/05/19

Test No: 972461


### Animal and Sample Description

**Animal Name:** Kentucky Bulleit  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 35140191  
**Sample Location:** Side  
**Sample Date:** 05/13/18  
**Age:** 06/12/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.9 microns	<b>Spin Fineness:</b>	16.9 microns
<b>Standard Deviation:</b>	3.1 microns	<b>Mean Curvature (deg/mm):</b>	50.3
<b>Coefficient of Variation:</b>	17.3 %	<b>SD Curvature (deg/mm):</b>	27.5
<b>Fibers Greater Than 30 microns:</b>	0.3 %	<b>Comfort Factor:</b>	99.7 %

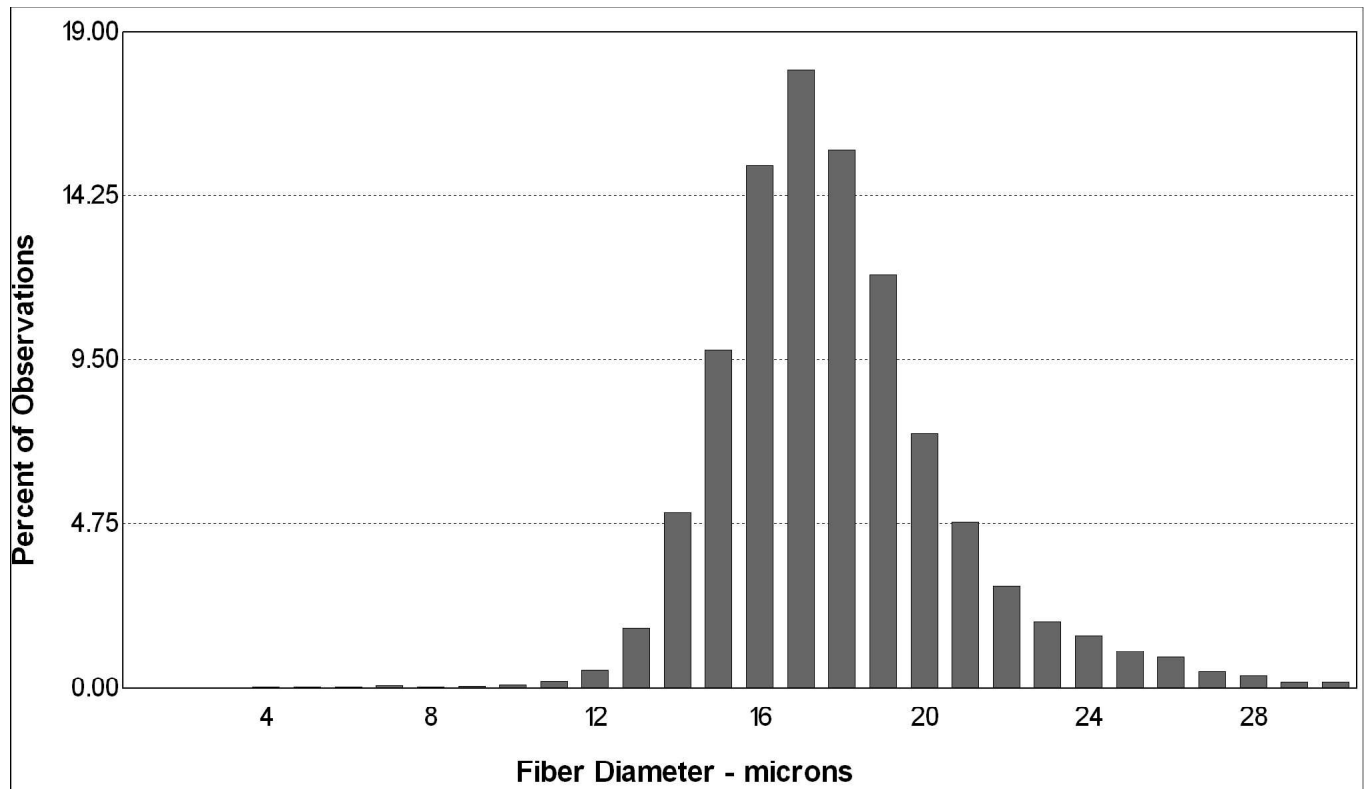

This Test Performed According to I.W.T.O Method 47