

Yocom-McColl Testing Laboratories, Inc.  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA 100)  
Micron Test Report**

Snowmass Alpacas LLC/Don & Julie Skinner  
270 Rapid Lightning Road  
Sandpoint ID 83864-4746 USA

**Date:** 08/04/14  
**Test No:** 484137


**Animal and Sample Description**

**Animal Name:** Snowmass Arch Angel XX  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 32726220  
**Sample Location:** Grid  
**Sample Date:** 05/17/14  
**Age:** 06/21/13

**Laboratory Data**

<b>Mean Fiber Diameter:</b>	12.6 microns	<b>Fibers Greater Than 30 microns:</b>	0.2 %
<b>Standard Deviation:</b>	2.4 microns	<b>Comfort Factor:</b>	99.8 %
<b>Coefficient of Variation:</b>	19.1 %	<b>Mean Curvature:</b>	46.1 deg/mm
<b>Spin Fineness:</b>	12.1 microns	<b>SD Curvature:</b>	31.1 deg/mm

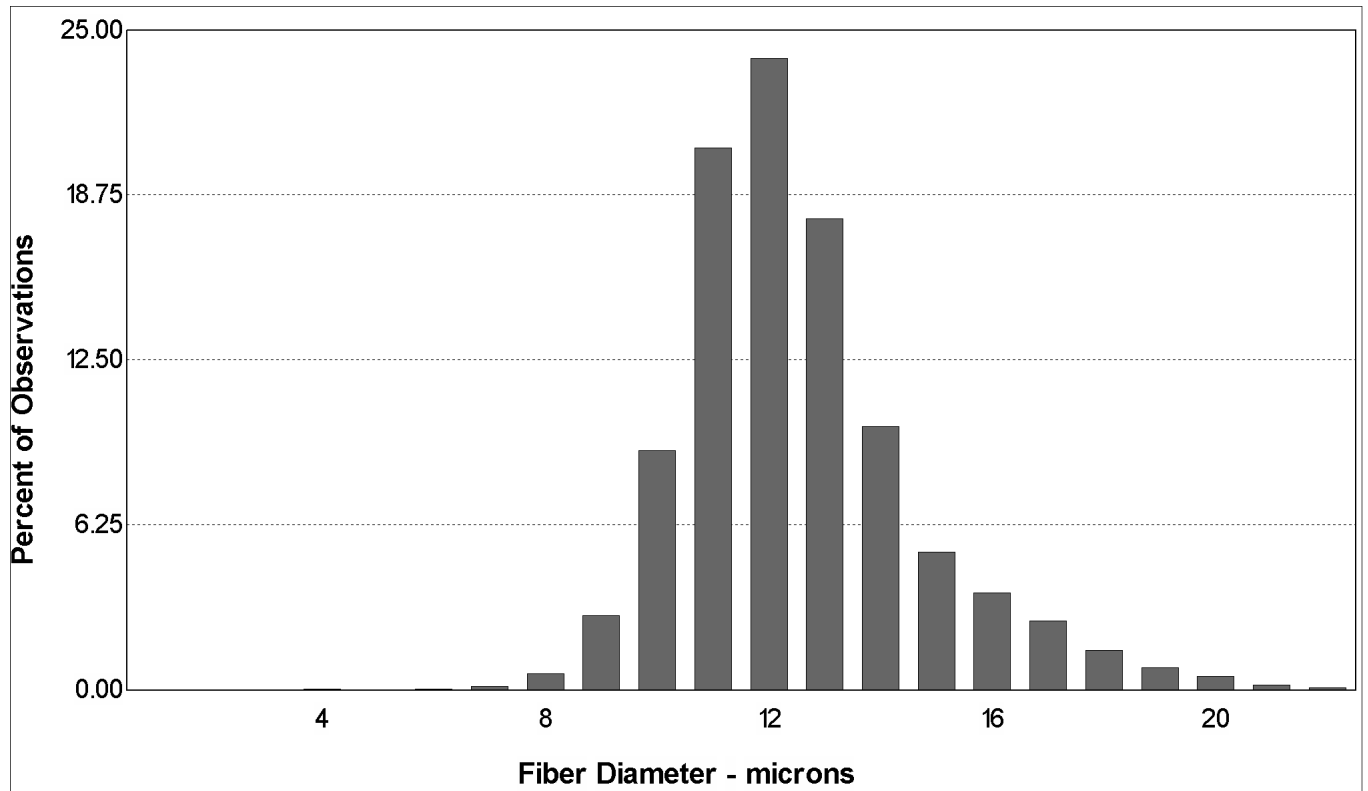

This Test Performed According to I.W.T.O Method 47