



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Anderson Acres Alpacas, LLC/Roy Anderson  
8812 S 230 Plaza Circle  
Gretna NE 68028 USA

04/08/19

Test No: 973418


### Animal and Sample Description

**Animal Name:** ANDACAL Anvil's Skyfyre  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Dark Fawn

**Animal ID:** 35418191  
**Sample Location:** Side  
**Sample Date:** 03/28/19  
**Age:** 07/03/18

### Laboratory Data

**Mean Fiber Diameter:** 18.9 microns  
**Standard Deviation:** 6.0 microns  
**Coefficient of Variation:** 31.8 %  
**Fibers Greater Than 30 microns:** 6.6 %

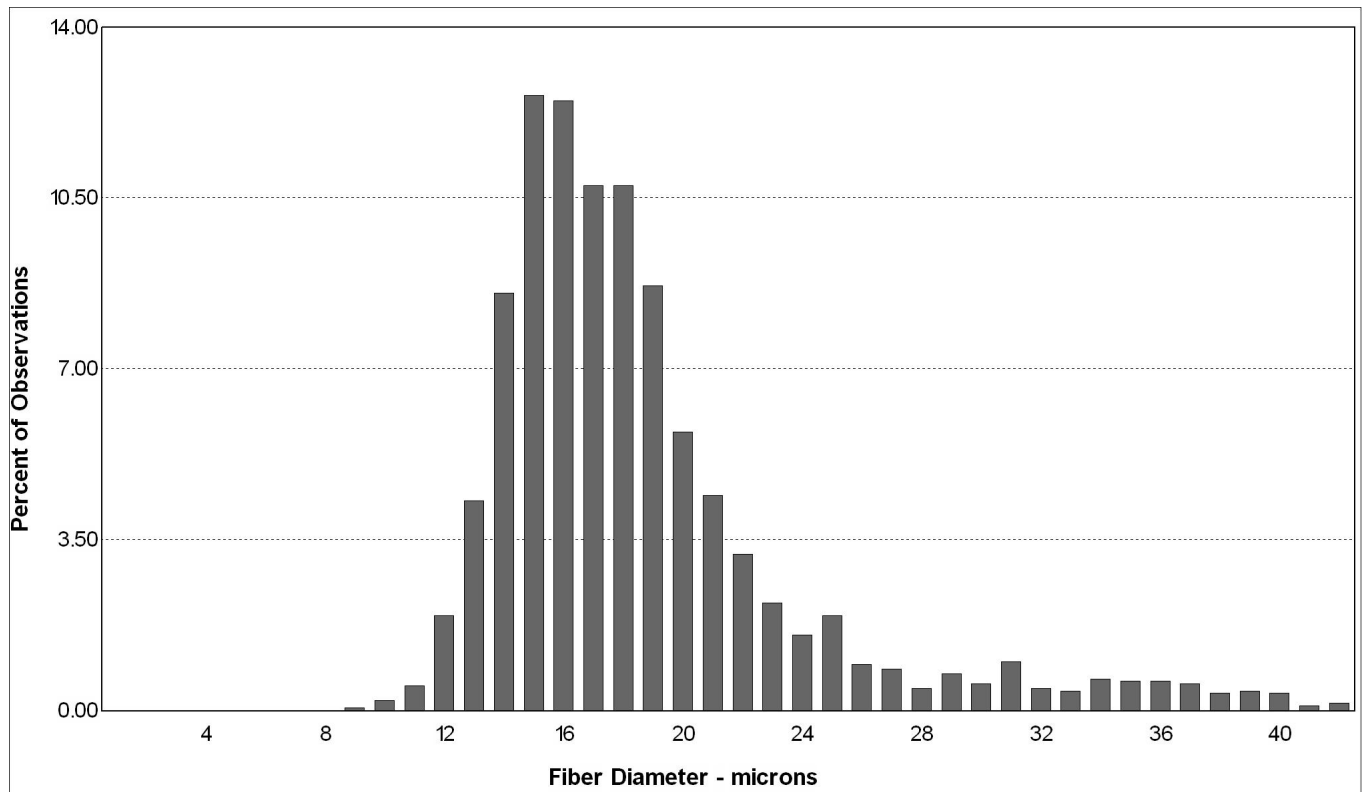

This Test Performed According to I.W.T.O Method 12