



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Hasselbring's Harmony Ranch/Patty Hasselbring  
29049 Davis Road  
Concordia MO 64020 USA

**Date:** 07/17/18  
**Shear ID:** 169483  
**Test No:** 963645


### Animal and Sample Description

**Animal Name:** Argento's Moonbeam of Harmony  
**ARI #:** 35082361  
**Breed:** Alpaca(Suri)  
**Sex:** Female  
**Color:** Lt Fawn

**Date of Birth (Age):** 07/22/16  
**Sample Location:** Side  
**Sample Date:** 05/21/18  
**Previous Shear Date:** 05/19/17  
**Total Fleece Wt (lbs):** 6.80

### Laboratory Data

<b>Mean Fiber Diameter:</b>	21.1 microns	<b>Mean Staple Length:</b>	170.6 mm
<b>Standard Deviation:</b>	5.7 microns	<b>Length Standard Deviation:</b>	7.1 mm
<b>Coefficient of Variation:</b>	27.0 %	<b>Length Coefficient of Variation:</b>	4.2 %
<b>Spin Fineness:</b>	21.8 microns	<b>Mean Curvature:</b>	11.7 deg/mm
<b>Fibers Greater Than 30 microns:</b>	5.9 %	<b>SD Curvature:</b>	16.5 deg/mm
<b>Comfort Factor:</b>	94.1 %		

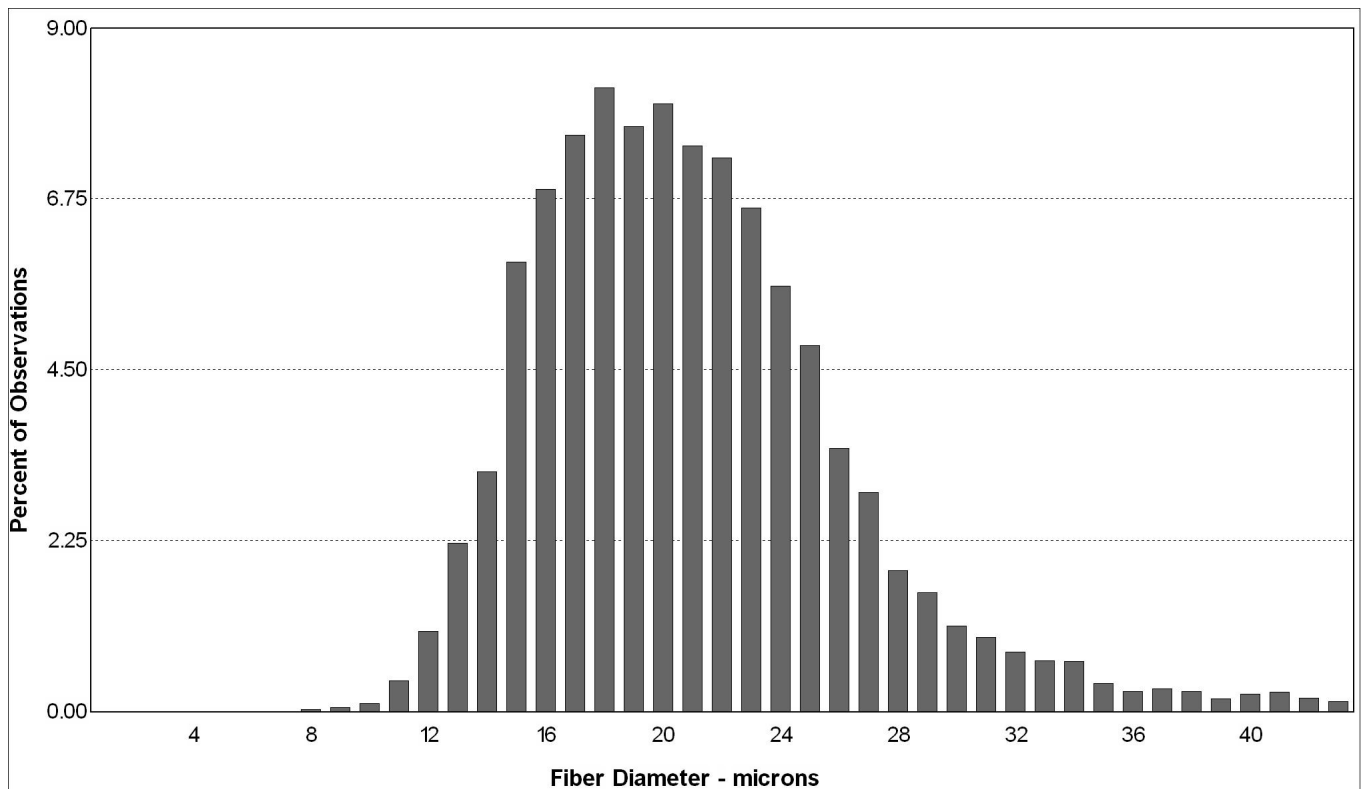

This Test Performed According to I.W.T.O Method 47