



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Crane Creek Ranch Alpacas/Brian Cunningham
1100 State Hwy A
Crane MO 65633 USA

04/30/19

Test No: 974167


Animal and Sample Description

Animal Name: Crane Creek's Gypsy
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/20/19
Age: 03/19/19 (1 Mo)

Laboratory Data

Mean Fiber Diameter: 18.8 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 24.1 %
Fibers Greater Than 30 microns: 2.7 %

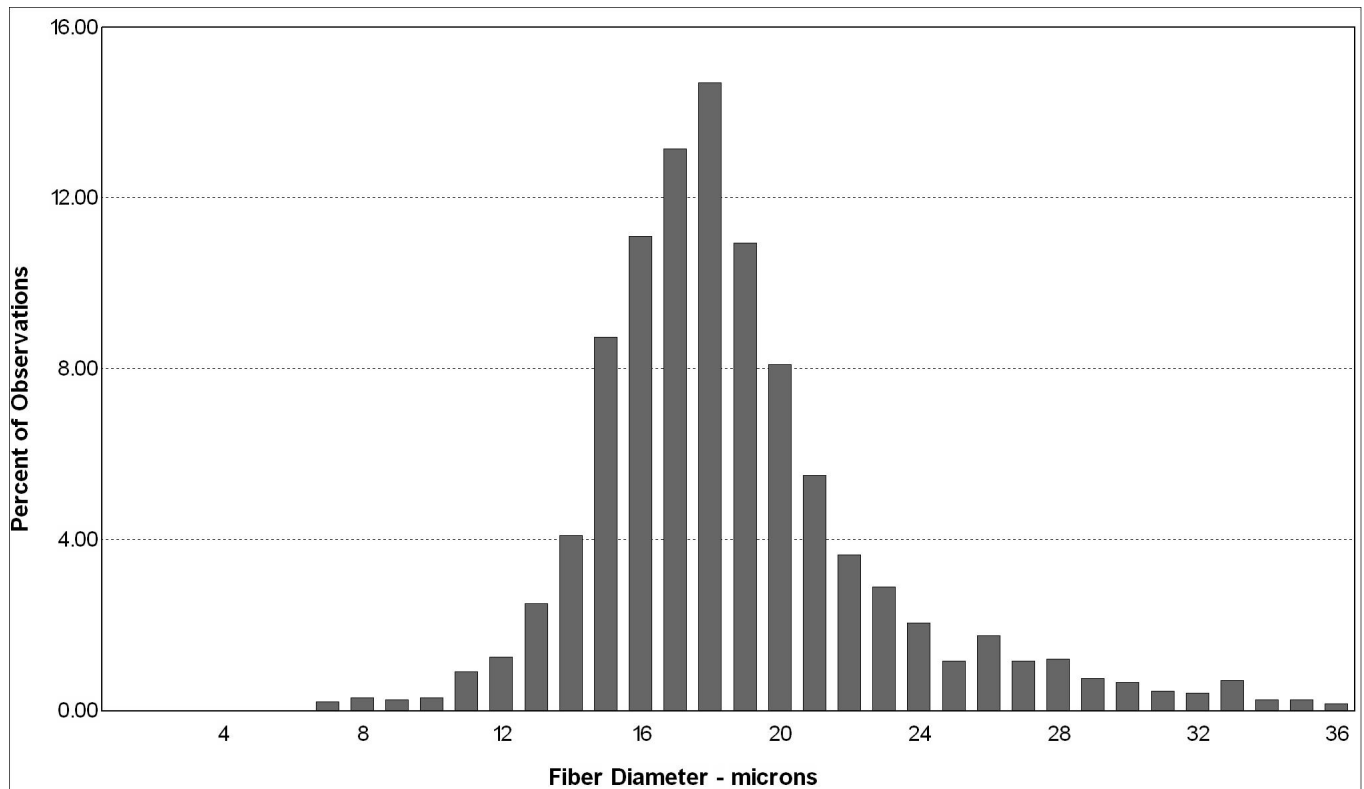

This Test Performed According to I.W.T.O Method 12