



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

B I Bar Ranch/Ted & Julie Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

07/22/19

Test No: 978576


Animal and Sample Description

Animal Name: Belle Starr
Breed: Alpaca(Suri)
Sex: Female
Color: Fawn

Animal ID: 35410881
Sample Location: Mid Side
Sample Date: 05/27/19
Age: 07/02/17

Laboratory Data

Mean Fiber Diameter: 21.6 microns
Standard Deviation: 4.3 microns
Coefficient of Variation: 20.0 %
Fibers Greater Than 30 microns: 3.1 %

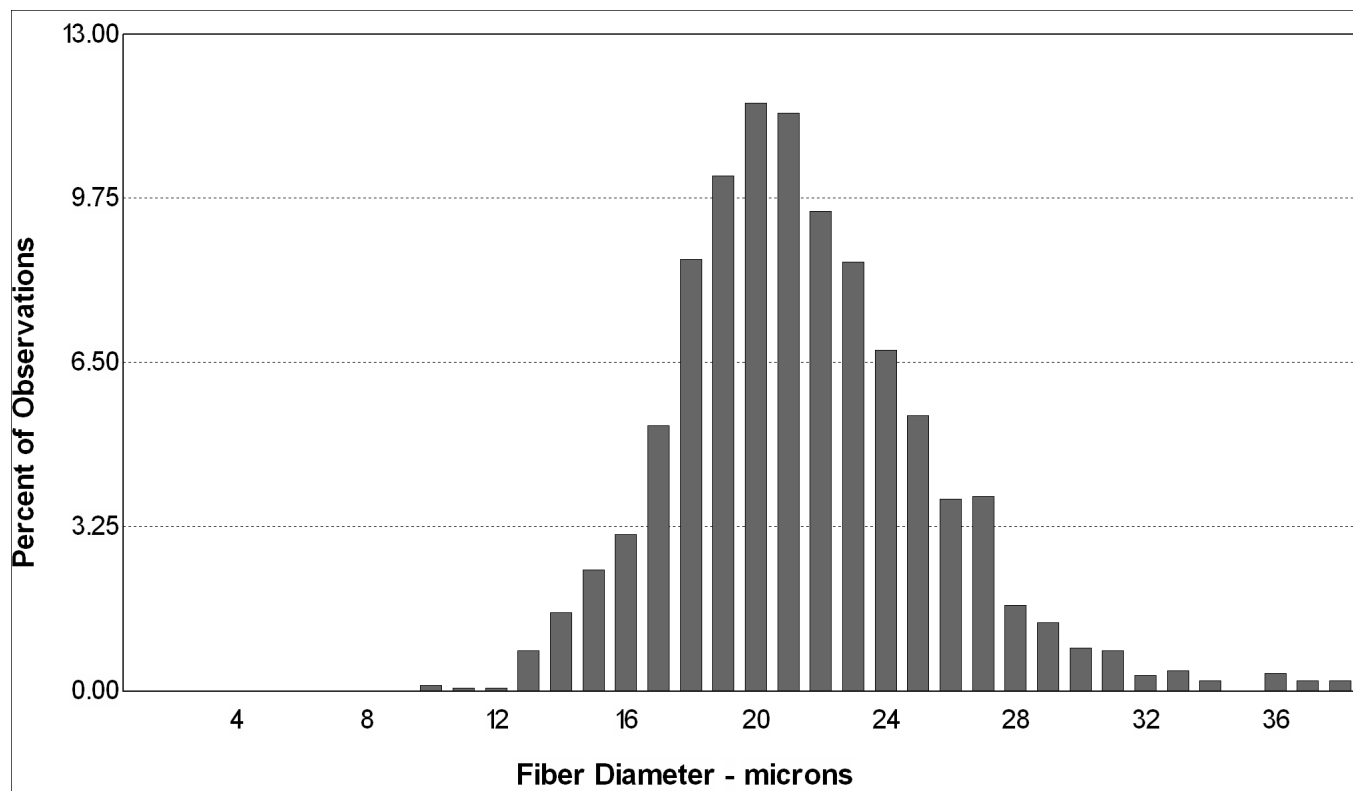

This Test Performed According to I.W.T.O Method 12