



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Plum Creek Alpacas/Brian B. Smith
8260 Plum Creek Way
Prescott Valley AZ 86315-9260 USA

Date: 07/22/19
Shear ID: 184570
Test No: 976855


Animal and Sample Description

Animal Name: Plum Creek's Rosa Sunrise
ARI #: 35466772
Breed: Alpaca(Huacaya)
Sex: Female
Color: Dark Brown

Date of Birth (Age): 09/13/18
Sample Location: Side
Sample Date: 04/17/19
Previous Shear Date: XX/XX/XX
Total Fleece Wt (lbs): 2.38

Laboratory Data

Mean Fiber Diameter:	18.1 microns	Mean Staple Length:	87.0 mm
Standard Deviation:	4.8 microns	Length Standard Deviation:	6.0 mm
Coefficient of Variation:	26.7 %	Length Coefficient of Variation:	6.9 %
Spin Fineness:	18.6 microns	Mean Curvature:	40.1 deg/mm
Fibers Greater Than 30 microns:	1.5 %	SD Curvature:	26.5 deg/mm
Comfort Factor:	98.5 %		

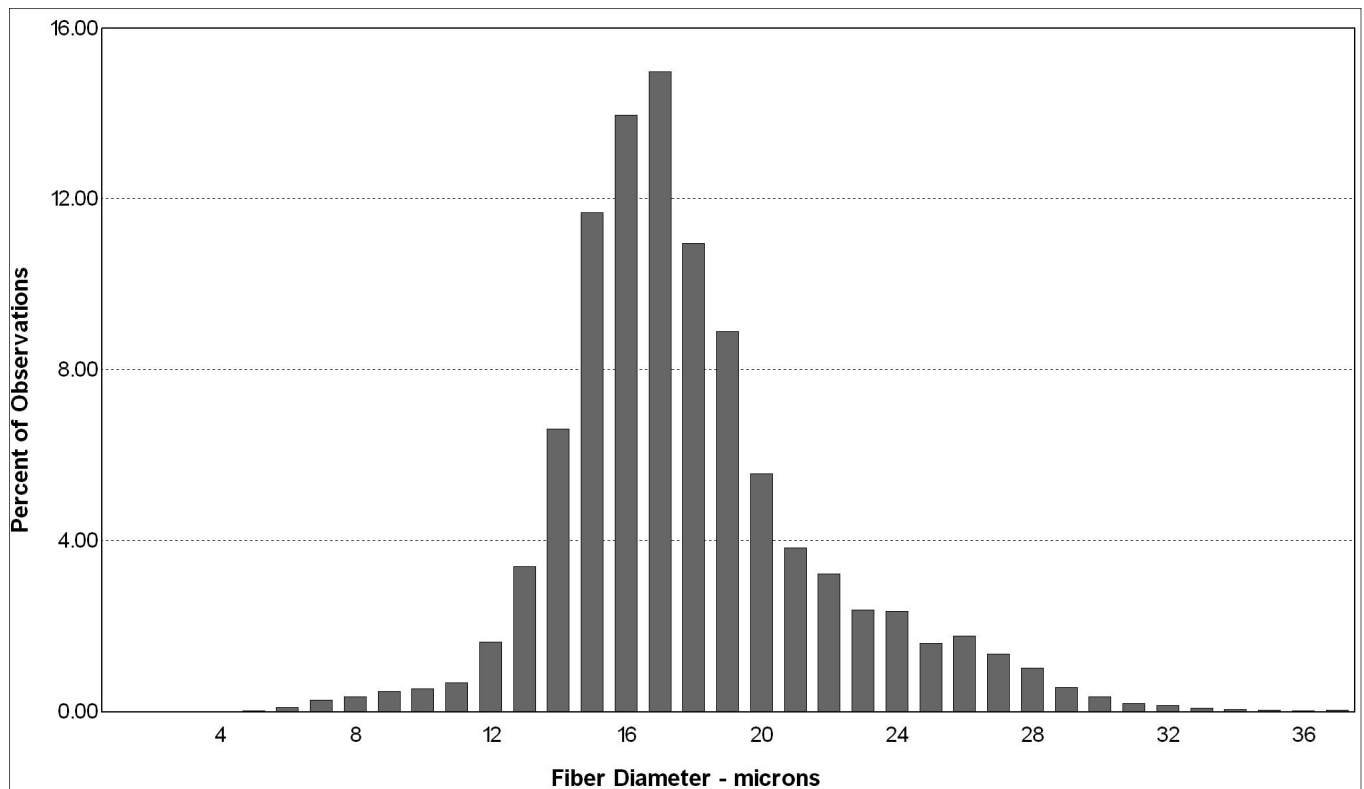

This Test Performed According to I.W.T.O Method 47