



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Thordarson Farms/Heather Thordarson
13492 South Warnock Rd
Oregon City OR 97045-9142 USA

Date: 08/16/19

Test No: 981041


Animal and Sample Description

Animal Name: NPA's Isabella
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 35413899
Sample Location: Mid Side
Sample Date: 06/09/19
Age: 08/23/18

Laboratory Data

Mean Fiber Diameter:	14.1 microns	Fibers Greater Than 30 microns:	0.3 %
Standard Deviation:	2.8 microns	Comfort Factor:	99.7 %
Coefficient of Variation:	19.6 %	Mean Curvature:	55.2 deg/mm
Spin Fineness:	13.6 microns	SD Curvature:	30.5 deg/mm

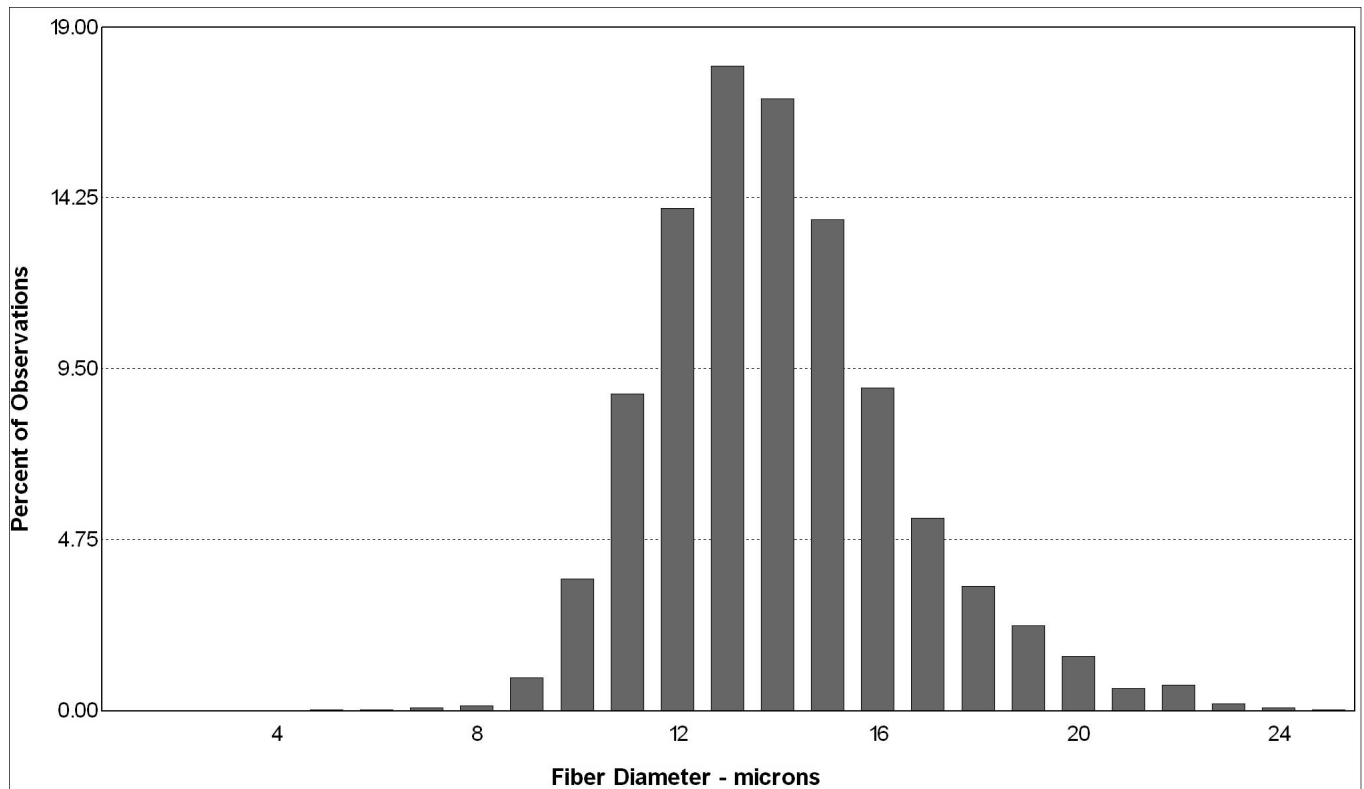

This Test Performed According to I.W.T.O Method 47