



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Pacesetter Alpacas/Dennis & Christy Pace  
5546 W Plymouth Church Rd  
Beloit WI 53511 USA

07/30/19

Test No: 979121


### Animal and Sample Description

Animal Name: Amazing Grace  
Breed: Alpaca(Suri)  
Sex: Female  
Color: Med Fawn

Animal ID: 31821513  
Sample Location: Side  
Sample Date: 05/06/19  
Age: 09/15/11

### Laboratory Data

Mean Fiber Diameter:	26.1 microns	Spin Fineness:	25.5 microns
Standard Deviation:	5.6 microns	Medullated Fibers:	0.0 %
Coefficient of Variation:	21.5 %	Mean Curvature (deg/mm):	8.1
Fibers Greater Than 30 microns:	16.8 %	SD Curvature (deg/mm):	9.7

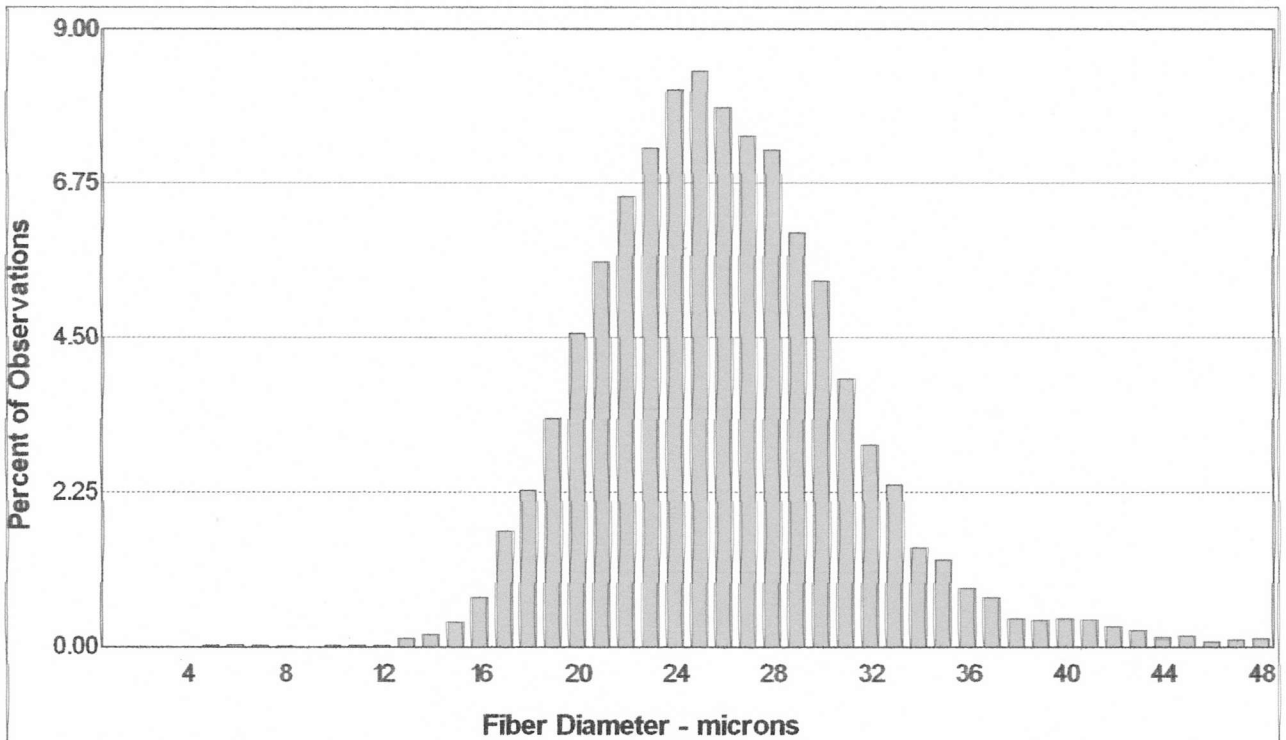

This Test Performed According to I.W.T.O Method 47