



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Rare Gem Alpacas/Darcy Phillips  
3507 W Stetson Ave #202  
Hemet CA 92545-9740 USA


**Date:** 09/19/19  
**Shear ID:** 194085  
**Test No:** 983458

### Animal and Sample Description

<b>Animal Name:</b>	Running Late's Peaches and Cream	<b>Date of Birth (Age):</b>	06/22/17
<b>ARI #:</b>	35369189	<b>Sample Location:</b>	Side
<b>Breed:</b>	Alpaca(Huacaya)	<b>Sample Date:</b>	04/24/19
<b>Sex:</b>	Female	<b>Previous Shear Date:</b>	05/18/18
<b>Color:</b>	Lt Fawn	<b>Total Fleece Wt (lbs):</b>	7.00

### Laboratory Data

<b>Mean Fiber Diameter:</b>	16.5 microns	<b>Mean Staple Length:</b>	73.2 mm
<b>Standard Deviation:</b>	3.8 microns	<b>Length Standard Deviation:</b>	4.6 mm
<b>Coefficient of Variation:</b>	22.8 %	<b>Length Coefficient of Variation:</b>	6.2 %
<b>Spin Fineness:</b>	16.3 microns	<b>Mean Curvature:</b>	51.0 deg/mm
<b>Fibers Greater Than 30 microns:</b>	0.8 %	<b>SD Curvature:</b>	30.2 deg/mm
<b>Comfort Factor:</b>	99.2 %		

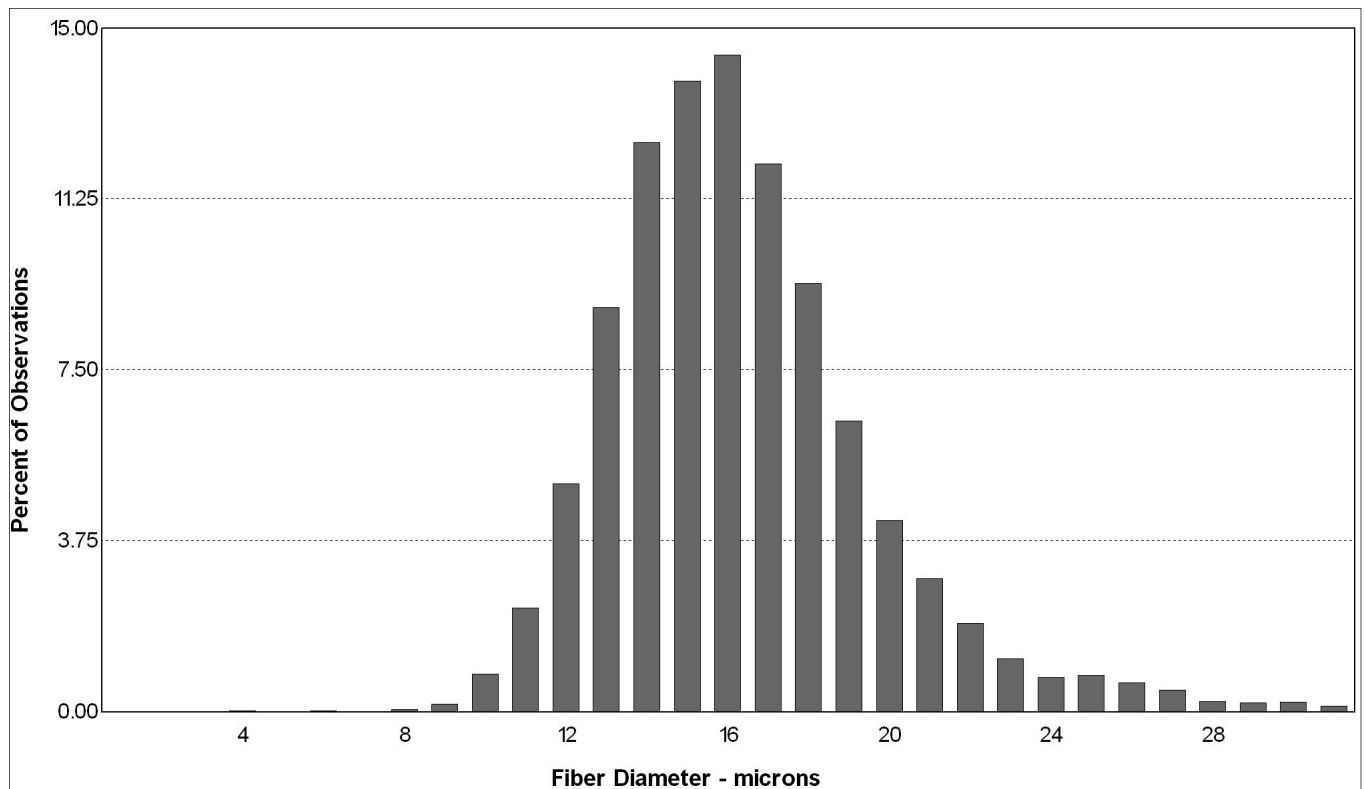

This Test Performed According to I.W.T.O Method 47