



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Wilkins Livestock Ranch/Mike & Janet Wilkins
1405 Rd 12
Geneva NE 68361 USA

10/23/19

Test No: 985906


Animal and Sample Description

Animal Name: WLK Vallisha
Breed: Alpaca(Suri)
Sex: Female
Color: Lt Brown

Animal ID: 36090099
Sample Location: Side (R)
Sample Date: 10/15/19
Age: XXXXX

Laboratory Data

Mean Fiber Diameter: 20.7 microns
Standard Deviation: 3.7 microns
Coefficient of Variation: 17.7 %
Fibers Greater Than 30 microns: 1.8 %

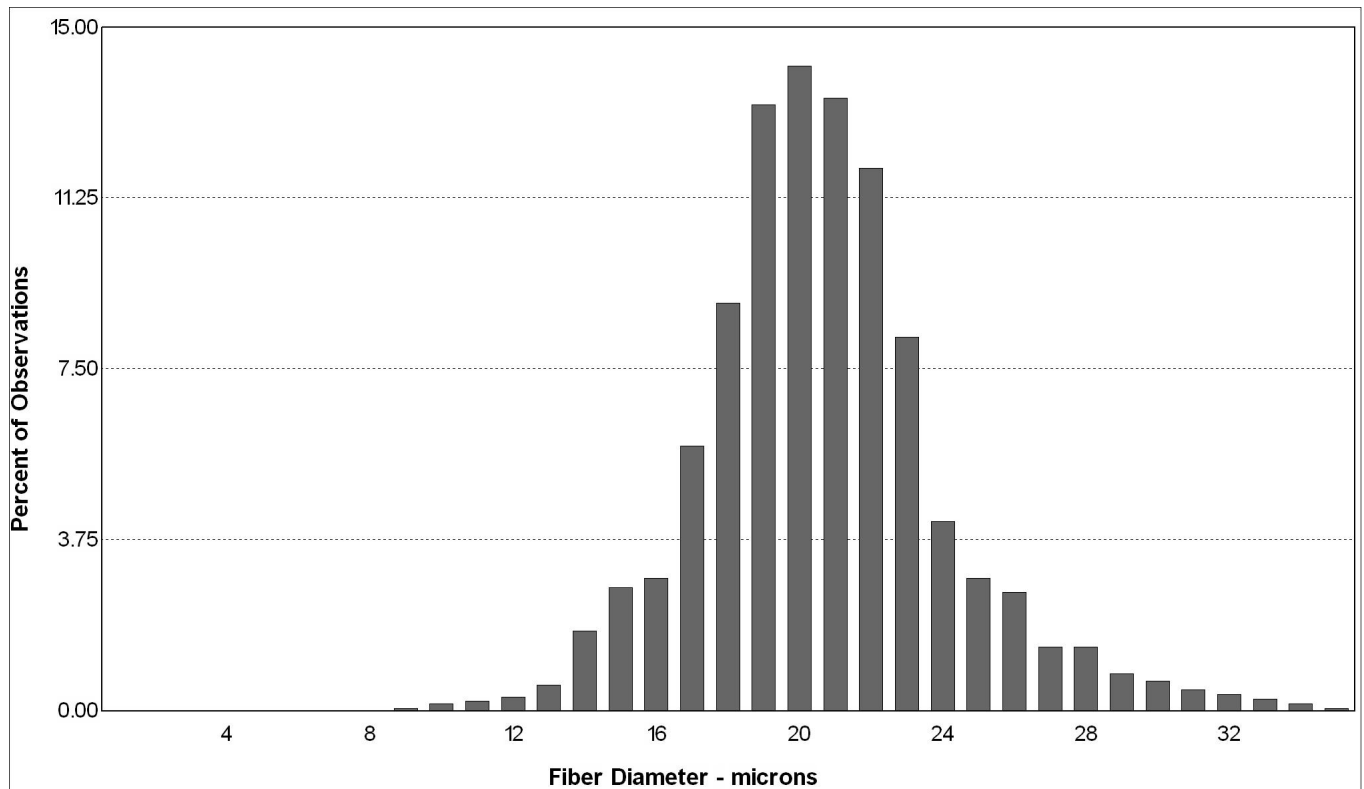

This Test Performed According to I.W.T.O Method 12