



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ten Seven Acres/Jessie Monson
107 Galchutt Ave
Galchutt ND 58075 USA

Date: 03/12/20

Test No: 987820


Animal and Sample Description

Animal Name: St. Pauli Girl
Breed: Alpaca(Huacaya)
Sex: Female
Color: Dark Rose Grey

Animal ID: XXXXX
Sample Location: Mid Side
Sample Date: 05/07/19
Age: 09/19/18

Laboratory Data

Mean Fiber Diameter:	20.0 microns	Fibers Greater Than 30 microns:	1.2 %
Standard Deviation:	3.6 microns	Comfort Factor:	98.8 %
Coefficient of Variation:	17.8 %	Mean Curvature:	35.7 deg/mm
Spin Fineness:	18.9 microns	SD Curvature:	20.9 deg/mm

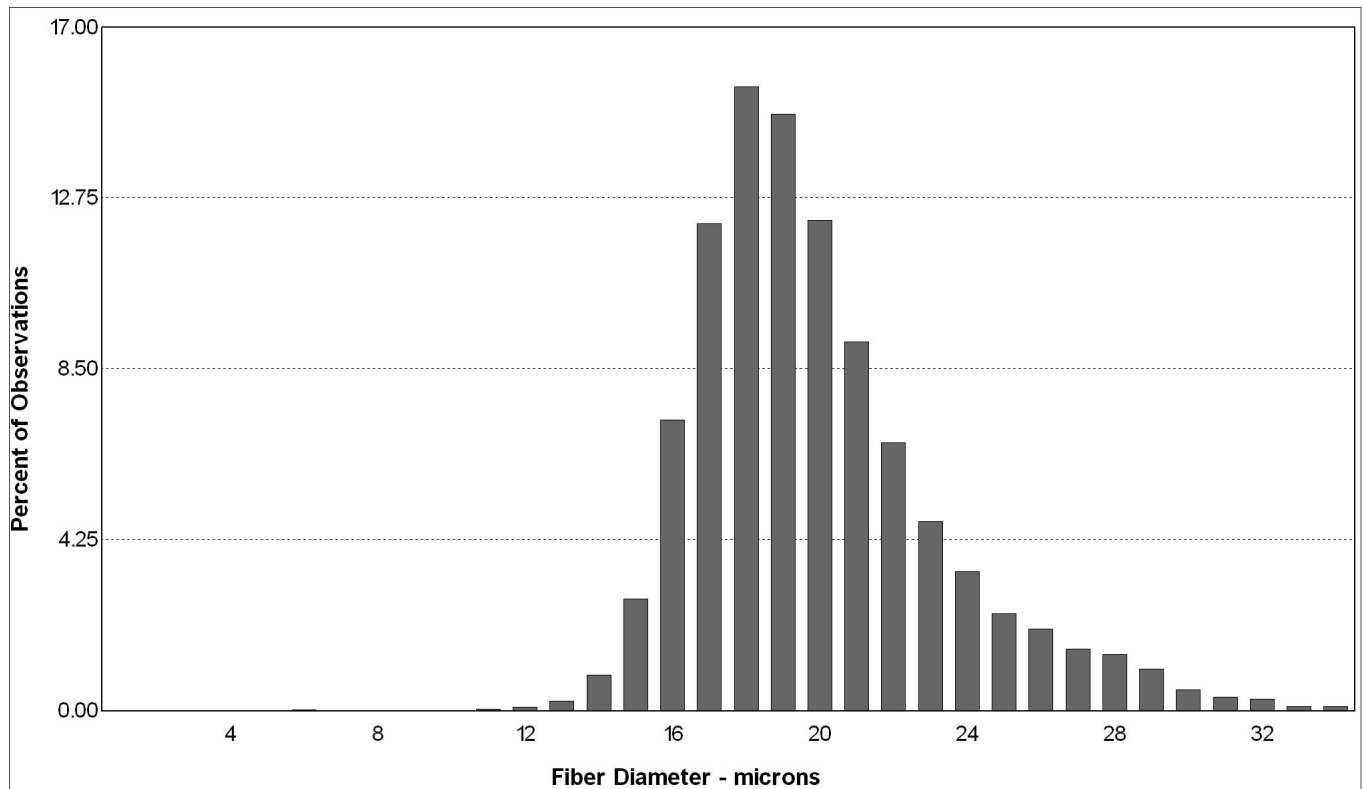

This Test Performed According to I.W.T.O Method 47