



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

ROCKSTAR Alpacas/Lisa Beatty  
16440 Bonney Road  
Watsonville CA 95076 USA

Date: 08/20/19

Test No: 981720


### Animal and Sample Description

**Animal Name:** ROCKSTAR's Revival  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 35597247  
**Sample Location:** Side  
**Sample Date:** 05/10/19  
**Age:** 12/19/18

### Laboratory Data

<b>Mean Fiber Diameter:</b>	14.3 microns	<b>Fibers Greater Than 30 microns:</b>	0.6 %
<b>Standard Deviation:</b>	4.3 microns	<b>Comfort Factor:</b>	99.4 %
<b>Coefficient of Variation:</b>	30.1 %	<b>Mean Curvature:</b>	37.6 deg/mm
<b>Spin Fineness:</b>	15.2 microns	<b>SD Curvature:</b>	23.7 deg/mm

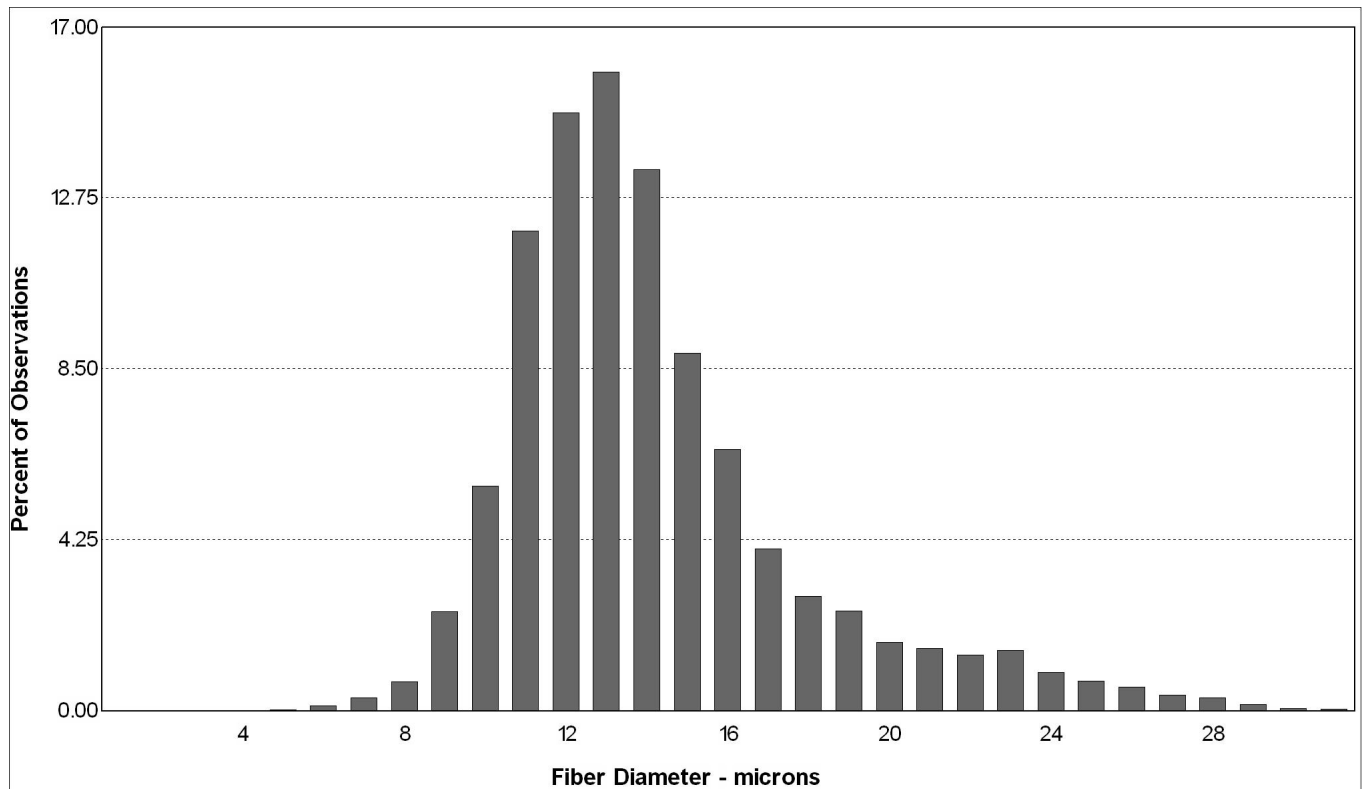

This Test Performed According to I.W.T.O Method 47