



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Olde Lyfe Alpacas/Stacey Payne  
500 Cleveland St  
Fallon NV 89406 USA

09/17/19

Test No: 983641


### Animal and Sample Description

**Animal Name:** Andina's Abigail  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** True Black

**Animal ID:** 35262411  
**Sample Location:** Side (L)  
**Sample Date:** 05/15/19  
**Age:** 06/06/14

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.0 microns	<b>Spin Fineness:</b>	22.3 microns
<b>Standard Deviation:</b>	4.7 microns	<b>Mean Curvature (deg/mm):</b>	34.3
<b>Coefficient of Variation:</b>	20.3 %	<b>SD Curvature (deg/mm):</b>	20.6
<b>Fibers Greater Than 30 microns:</b>	6.6 %	<b>Comfort Factor:</b>	93.4 %

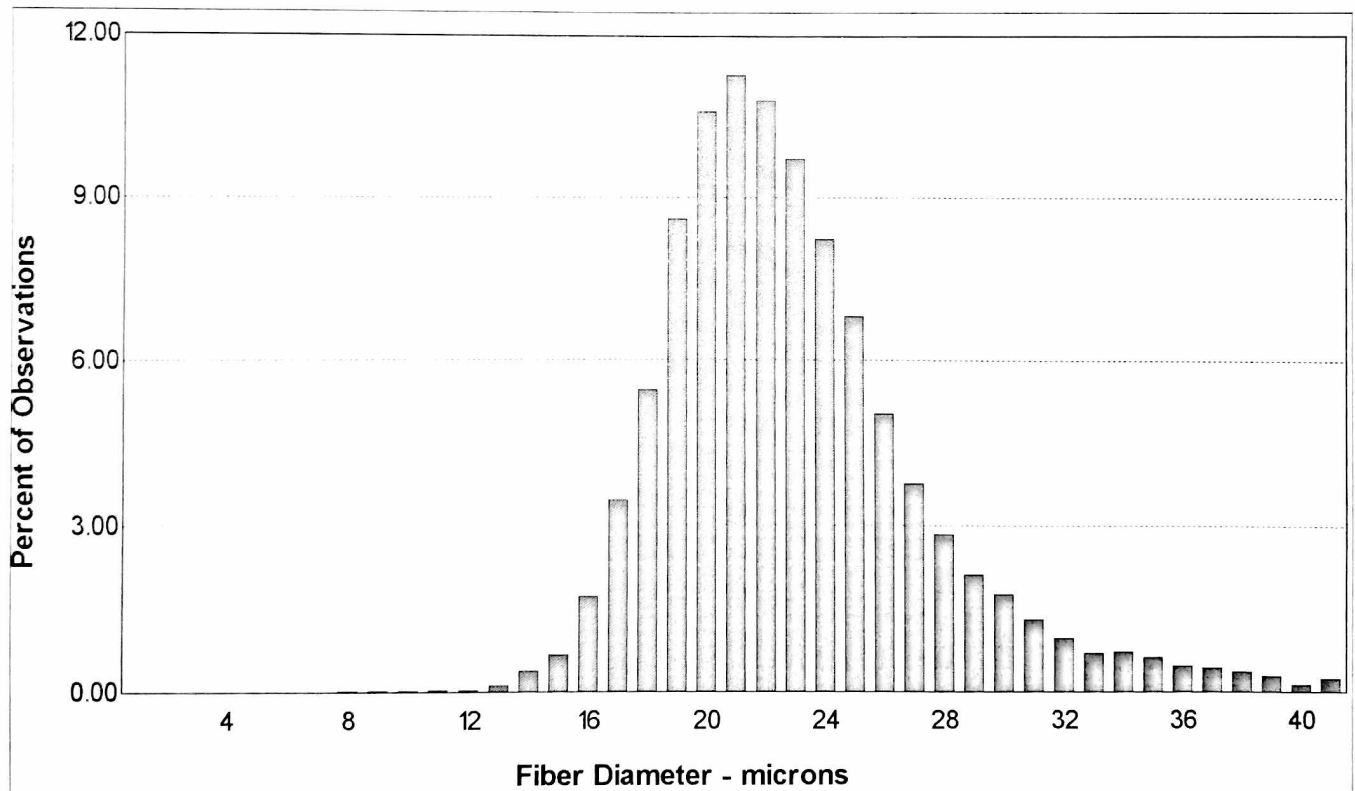

This Test Performed According to I.W.T.O Method 47