



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Brill Road
West Bolton QC J0E 2T0 Canada

Date: 07/12/19

Test No: 976960


Animal and Sample Description

Animal Name: Ariya Belenis' Antique Lace (Keaton's)
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Mid Side
Sample Date: 05/05/19
Age: 07/17/18

Laboratory Data

Mean Fiber Diameter:	13.6 microns	Fibers Greater Than 30 microns:	0.0 %
Standard Deviation:	2.8 microns	Comfort Factor:	100.0 %
Coefficient of Variation:	20.2 %	Mean Curvature:	58.2 deg/mm
Spin Fineness:	13.2 microns	SD Curvature:	34.7 deg/mm

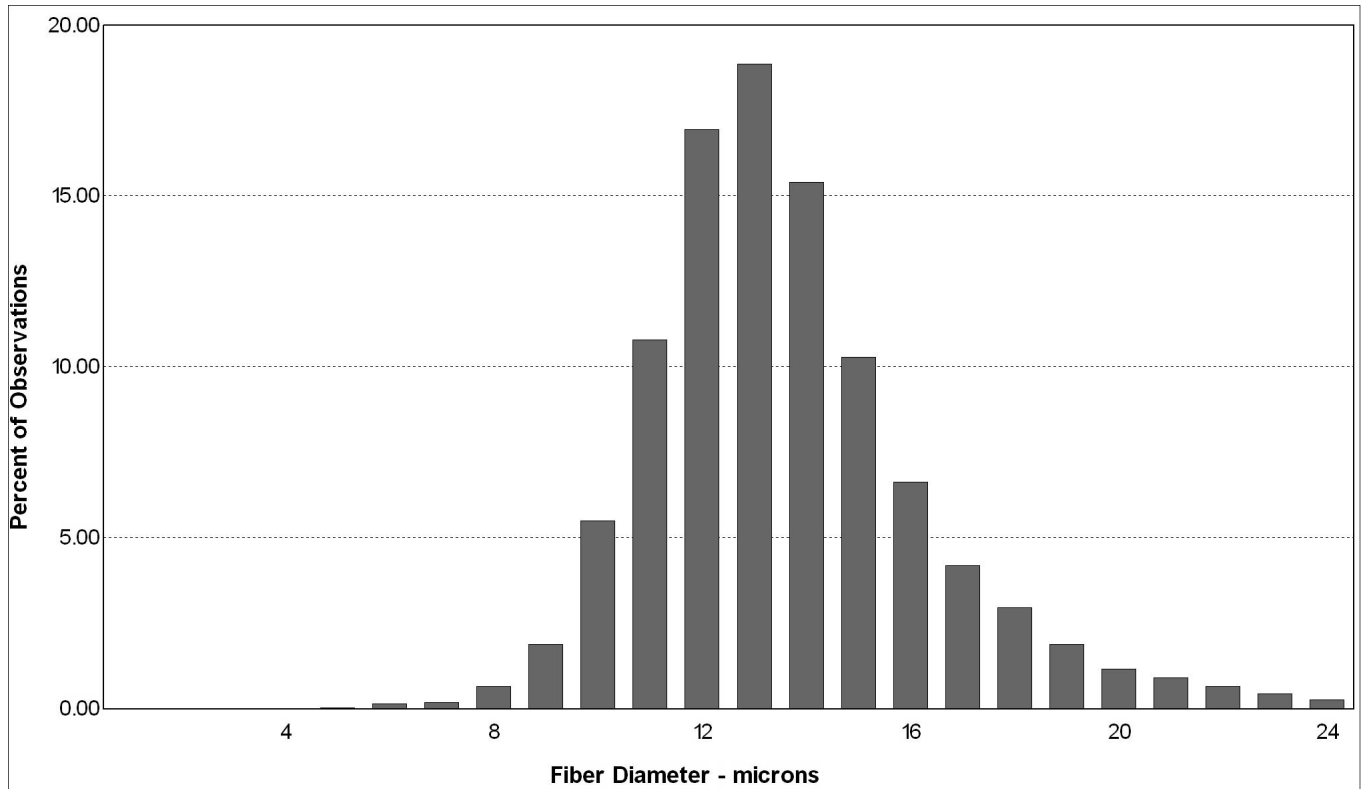

This Test Performed According to I.W.T.O Method 47